

# Technical Information

## Liquiline M CM42

Two-wire transmitter for hazardous and non-hazardous areas



Memosens: pH/ORP, oxygen, conductivity

Analog sensors: pH/ORP, conductivity, concentration, resistivity

### Application

Liquiline M CM42 is a two-wire transmitter for liquid analysis in all areas of process technology.

The very robust plastic version and the hygienic stainless steel version are perfectly tailored to the following applications:

- Chemical processes
- Pharmaceutical industry
- Food technology
- Applications in hazardous areas

The transmitter is suitable for pollution degree 3 according to IEC/EN 61010-1.

### Your benefits

- Cost-reducing:
  - Easy commissioning with Quick Setup and navigator
  - Memosens: plug & play with lab-calibrated sensors
  - Optimization of process and maintenance with sensor data
- Reduced inventory thanks to modular design
- Effective asset management with Fieldcare and W@M

*[Continued from front page]*

- Safe:
  - Memosens: Active indication of a cable break
  - User-guided commissioning, graphic display and plain-text guidance for maximum operating safety
  - Approvals: ATEX, IECEx, CSA, FM, NEPSI, Japan-Ex, EAC-Ex
  - User administration: Code-protected configuration

## Table of contents


<b>Function and system design</b> .....	<b>4</b>	<b>Power supply</b> .....	<b>15</b>
Measuring system .....	4	Supply voltage .....	15
<b>Equipment architecture</b> .....	<b>5</b>	Cable specification .....	15
Firmware .....	5	Grounding the housing .....	16
DAT memory modules .....	6	Power supply and signal circuit .....	17
Connectable sensors .....	6	Sensor connection .....	19
<b>Dependability</b> .....	<b>7</b>	<b>Performance characteristics</b> .....	<b>26</b>
Reliability .....	7	Response time of current output .....	26
Maintainability .....	8	Maximum measured error Memosens .....	26
Safety .....	9	Tolerance, current outputs .....	26
<b>Input</b> .....	<b>10</b>	Repeatability .....	26
Measured variables .....	10	Temperature compensation, conductivity .....	26
Measuring ranges .....	10	Temperature adjustment .....	26
<b>Binary input Memosens</b> .....	<b>10</b>	<b>Installation</b> .....	<b>27</b>
Cable specification .....	10	Installation conditions .....	27
Ex specification .....	10	Installation in hazardous areas .....	28
<b>Analog input pH/ORP</b> .....	<b>10</b>	Installation options .....	31
Cable specification .....	10	<b>Environment</b> .....	<b>31</b>
Temperature sensors .....	10	Ambient temperature .....	31
Ex specification .....	11	Storage temperature .....	31
Input impedance .....	11	Humidity .....	31
Input leak current .....	11	Degree of protection .....	32
<b>Analog input conductivity</b> .....	<b>11</b>	Electromagnetic compatibility .....	32
Cable specification .....	11	Degree of contamination .....	32
Temperature sensors .....	11	<b>Mechanical construction</b> .....	<b>32</b>
Ex specification, sensors with conductive measurement of conductivity .....	12	Dimensions .....	32
Ex specification, sensors with inductive measurement of conductivity .....	12	Weight .....	33
<b>Output</b> .....	<b>12</b>	Materials .....	33
Output signal .....	12	<b>Operability</b> .....	<b>34</b>
Signal on alarm .....	13	Operating concept .....	34
Load .....	13	Local operation .....	34
Output span .....	13	Language packages .....	35
Ex specification, current output .....	13	Remote operation .....	35
Ex specification PROFIBUS and FOUNDATION Fieldbus .....	13	<b>Certificates and approvals</b> .....	<b>37</b>
<b>Protocol-specific data</b> .....	<b>13</b>	CE mark .....	37
HART .....	13	Hazardous area approvals .....	37
PROFIBUS PA .....	14	Test reports .....	37
FOUNDATION Fieldbus .....	14	Other standards and guidelines .....	37
<b>Current output, passive</b> .....	<b>14</b>	<b>Ordering information</b> .....	<b>37</b>
Span .....	14	Product page .....	37
Signal characteristics .....	14	Product Configurator .....	37
Cable specification .....	14	Scope of delivery .....	37
		<b>Accessories</b> .....	<b>37</b>
		Device-specific accessories .....	38
		Communication-specific accessories .....	43
		Service-specific accessories .....	44
		System components .....	44

## Function and system design

### Measuring system

A complete measuring system comprises:

- Liquiline M CM42 transmitter with mounting plate (e.g. for wall mounting)
- Sensor and suitable sensor cable
- The following are optional:
  - Suitable probe holder
  - Post retainer
  - Weather protection cover

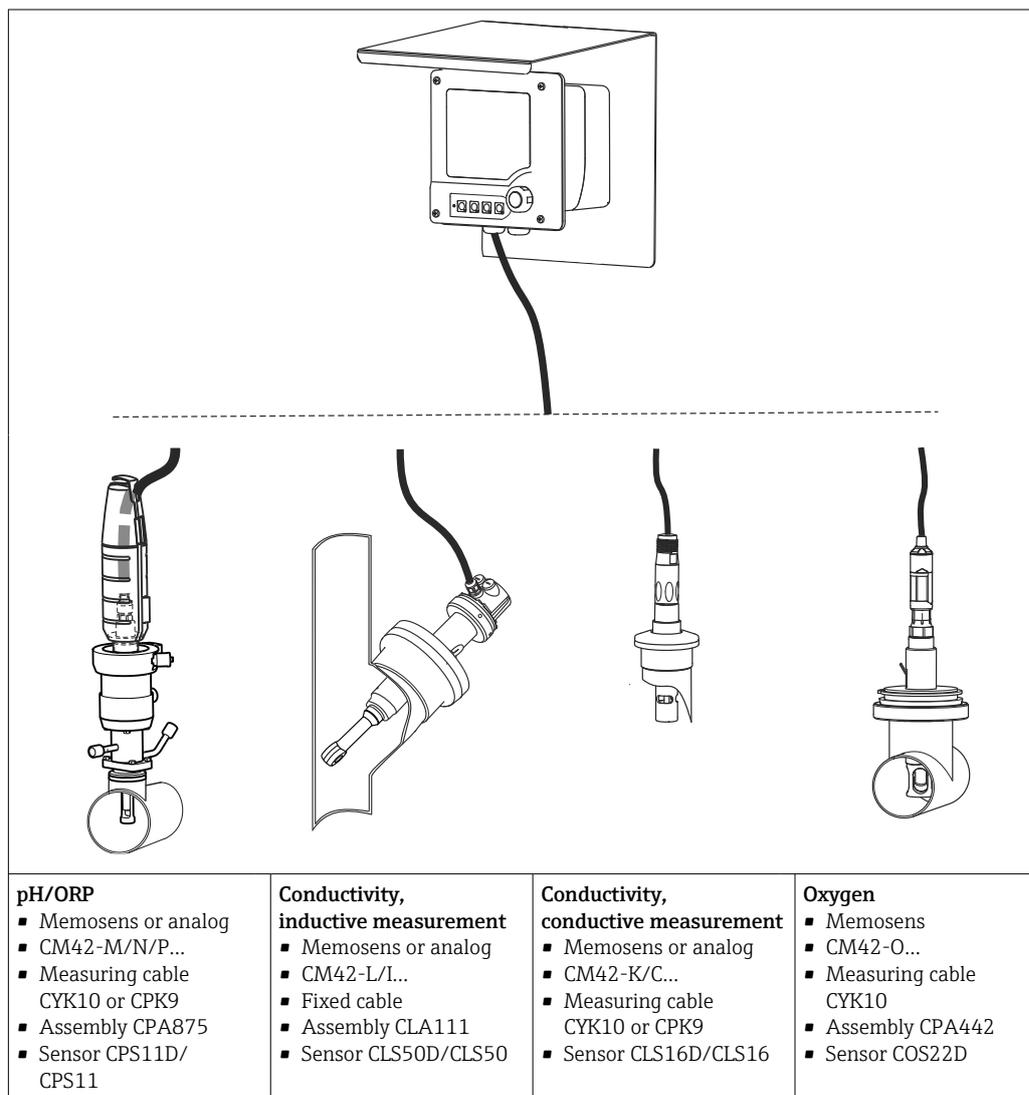

You can combine your measuring point with a variety of assemblies and sensors → 37. For more information, visit: [www.endress.com/cm42](http://www.endress.com/cm42)

#### NOTICE

#### Effect of climatic conditions: rain, snow, direct sunlight

Device damage to total device failure is possible!

- ▶ When installing outside, always use the weather protection cover. (→ 38)

## Equipment architecture

### Firmware

You can select the following from these software packages:

- Basic version (CM42-\*\*\*\*\*EA)  
Standard application for the most common measuring points
- Advanced version (CM42-\*\*\*\*\*EB)  
Many additional functions that increase the safety and quality
- Advanced features (CM42-\*\*\*\*\*EH)  
Additionally with measuring point monitor, overview of operating data

Package	Features					
	pH/ORP (glass/ISFET)	Conductivity	Oxygen			
Standard version	<p><b>Analog sensors</b></p> <ul style="list-style-type: none"> <li>■ Offset and two-point calibration</li> <li>■ Sample calibration</li> <li>■ Calibration with standard buffers</li> <li>■ Manual buffer specification</li> <li>■ Temperature compensation</li> <li>■ Temperature adjustment</li> <li>■ Isotherm intersection</li> <li>■ Simulation current output</li> <li>■ Self diagnostic</li> <li>■ Calibration stability settings</li> <li>■ Clock</li> </ul> <p><b>Memosens sensors</b> Like analog sensors and additionally:</p> <ul style="list-style-type: none"> <li>■ Sensor information</li> <li>■ Sensor check</li> </ul>	<p><b>Analog sensors</b></p> <ul style="list-style-type: none"> <li>■ Sample calibration</li> <li>■ Temperature calibration: Single-point</li> <li>■ Temperature compensation: Linear, NaCl, ultrapure water (NaCl, HCl)</li> <li>■ Simulation current output</li> <li>■ Self diagnostic</li> <li>■ Concentration measurement</li> <li>■ Clock</li> </ul> <p><b>Memosens sensors</b> Like analog sensors and additionally:</p> <ul style="list-style-type: none"> <li>■ Sensor information</li> <li>■ Sensor check</li> </ul>	<p><b>Memosens sensors</b></p> <ul style="list-style-type: none"> <li>■ Slope calibration <ul style="list-style-type: none"> <li>■ In air (100% RH)</li> <li>■ In water (100% air-saturated)</li> </ul> </li> <li>■ In air (specifying the current absolute air pressure and the relative humidity)</li> <li>■ Zero point calibration</li> <li>■ Sample calibration</li> <li>■ Temperature adjustment</li> <li>■ Medium compensation</li> <li>■ Calibration stability settings</li> <li>■ Simulation current output</li> <li>■ Self diagnostic</li> <li>■ Clock</li> <li>■ Sensor information</li> <li>■ Sensor check</li> </ul>			
Advanced version	<p><b>"Basic version" software package and additionally:</b></p> <table border="0" style="width: 100%;"> <tr> <td style="vertical-align: top; width: 33%;"> <p><b>Analog sensors</b></p> <ul style="list-style-type: none"> <li>■ Medium compensation</li> <li>■ Calibration timer</li> <li>■ Sensor condition check (SCC)</li> </ul> <p><b>Memosens sensors</b> Like analog sensors and additionally:</p> <ul style="list-style-type: none"> <li>■ Operating hours counter</li> <li>■ Sterilization counter</li> </ul> </td> <td style="vertical-align: top; width: 33%;"> <p><b>Analog sensors</b></p> <ul style="list-style-type: none"> <li>■ Calibration with separate installation factor (only inductive measurement)</li> <li>■ Polarization detection (only conductive measurement)</li> <li>■ Temperature compensation via user table</li> <li>■ Two-point temperature adjustment: offset and slope</li> <li>■ USP alarm and pre-alarm</li> </ul> <p><b>Memosens sensors</b> Like analog sensors and additionally:</p> <ul style="list-style-type: none"> <li>■ Operating hours counter</li> <li>■ Sterilization counter</li> </ul> </td> <td style="vertical-align: top; width: 33%;"> <p><b>Memosens sensors</b></p> <ul style="list-style-type: none"> <li>■ Configuration of polarization voltage</li> <li>■ Calibration timer</li> <li>■ Sensor statistics</li> <li>■ Operating hours counter</li> <li>■ Sterilization counter</li> </ul> </td> </tr> </table> <p>All devices, regardless of measuring parameter:</p> <ul style="list-style-type: none"> <li>■ Logbooks</li> <li>■ Data logbook</li> <li>■ Free assignment of measured values to current outputs (optional)</li> <li>■ Diagnostic function switch-on/off</li> <li>■ Advanced user administration</li> <li>■ Current output tables</li> </ul>			<p><b>Analog sensors</b></p> <ul style="list-style-type: none"> <li>■ Medium compensation</li> <li>■ Calibration timer</li> <li>■ Sensor condition check (SCC)</li> </ul> <p><b>Memosens sensors</b> Like analog sensors and additionally:</p> <ul style="list-style-type: none"> <li>■ Operating hours counter</li> <li>■ Sterilization counter</li> </ul>	<p><b>Analog sensors</b></p> <ul style="list-style-type: none"> <li>■ Calibration with separate installation factor (only inductive measurement)</li> <li>■ Polarization detection (only conductive measurement)</li> <li>■ Temperature compensation via user table</li> <li>■ Two-point temperature adjustment: offset and slope</li> <li>■ USP alarm and pre-alarm</li> </ul> <p><b>Memosens sensors</b> Like analog sensors and additionally:</p> <ul style="list-style-type: none"> <li>■ Operating hours counter</li> <li>■ Sterilization counter</li> </ul>	<p><b>Memosens sensors</b></p> <ul style="list-style-type: none"> <li>■ Configuration of polarization voltage</li> <li>■ Calibration timer</li> <li>■ Sensor statistics</li> <li>■ Operating hours counter</li> <li>■ Sterilization counter</li> </ul>
<p><b>Analog sensors</b></p> <ul style="list-style-type: none"> <li>■ Medium compensation</li> <li>■ Calibration timer</li> <li>■ Sensor condition check (SCC)</li> </ul> <p><b>Memosens sensors</b> Like analog sensors and additionally:</p> <ul style="list-style-type: none"> <li>■ Operating hours counter</li> <li>■ Sterilization counter</li> </ul>	<p><b>Analog sensors</b></p> <ul style="list-style-type: none"> <li>■ Calibration with separate installation factor (only inductive measurement)</li> <li>■ Polarization detection (only conductive measurement)</li> <li>■ Temperature compensation via user table</li> <li>■ Two-point temperature adjustment: offset and slope</li> <li>■ USP alarm and pre-alarm</li> </ul> <p><b>Memosens sensors</b> Like analog sensors and additionally:</p> <ul style="list-style-type: none"> <li>■ Operating hours counter</li> <li>■ Sterilization counter</li> </ul>	<p><b>Memosens sensors</b></p> <ul style="list-style-type: none"> <li>■ Configuration of polarization voltage</li> <li>■ Calibration timer</li> <li>■ Sensor statistics</li> <li>■ Operating hours counter</li> <li>■ Sterilization counter</li> </ul>				

Package	Features		
	pH/ORP (glass/ISFET)	Conductivity	Oxygen
Advanced features	<p><b>"Advanced version" software package and additionally:</b></p> <p>Measuring point operating data:</p> <ul style="list-style-type: none"> <li>▪ MTBF (mean time between failures), MTBC (mean time between calibrations), MTR (mean time to repair)</li> <li>▪ Measuring point operating time</li> <li>▪ Number of failures</li> <li>▪ Failure time</li> <li>▪ Availability</li> <li>▪ Process check system (PCS)</li> </ul>		

### DAT memory modules

There are 3 different types of DAT modules that can either be ordered as optional accessories or are already included in the delivery:

- **SystemDAT**

Sensor type replacement, firmware updates (more recent firmware version) or change of language group

- **FunctionDAT**

Extension of function range ("Advanced version" firmware or 2nd current output)

Upgrade to "Advanced functions" not possible

- **CopyDAT**

Memory for own configuration settings

### Device extensibility

- ▶ Before ordering a FunctionDAT, check if it is possible to extend the functional range of your device.

### Connectable sensors

#### pH/ORP

- Memosens and analog glass electrodes
- Memosens and analog ISFET sensors
- Memosens and analog ORP electrodes
- Memosens pH/ORP combined sensors
- Memosens and analog enamel pH electrodes
- Analog single electrodes (glass or antimony)

#### Conductivity

- Memosens and analog sensors, conductive measurement of conductivity
  - Two-electrode sensors
  - Four-electrode sensors
- Memosens and analog sensors, inductive measurement of conductivity

#### Oxygen

Amperometric and optical sensors:

- Memosens technology
- in 12 mm and 40 mm design

# Dependability

## Reliability

### Memosens

Memosens makes your measuring point safer and more reliable:

- Non-contact, digital signal transmission enables optimum galvanic isolation
- Sensor can be calibrated in a lab, thus increasing the availability of the measuring point in the process
- Intrinsically safe electronics mean operation in hazardous areas is not a problem.
- Predictive maintenance thanks to recording of sensor data, e.g.:
  - Total hours of operation
  - Hours of operation with very high or very low measured values
  - Hours of operation at high temperatures
  - Number of steam sterilizations
  - Sensor condition

Completely watertight

- Can even be connected under water
- No contact corrosion

### Quick Setup

#### To the first measured value within 1 minute

Once you have configured the few parameters in the Quick Setup menu, the measuring point is ready to measure. The first measured value is reliably displayed.

### Sensor Condition Check (SCC, only pH)

This function monitors the condition of the electrode and the degree of electrode aging. The status is indicated by the messages **SCC electrode sufficient** or **SCC electrode cond. bad**. The condition of the electrode is updated after every calibration.

### Sensor Check System (SCS, pH only)

The Sensor Check System (SCS) monitors the high impedance of the pH glass. An alarm is issued if a minimum impedance value is undershot or a maximum impedance is exceeded.


- Glass breakage is the main reason for a drop in high impedance values
- The reasons for increasing impedance values include:
  - Dry sensor
  - Worn pH glass membrane

### Process Check System (PCS): Life check ("Advanced features" firmware version only)

The process check system (PCS) checks the measuring signal for stagnation. An alarm is triggered if the measuring signal does not change over a specific period (several measured values).

The main causes of stagnating measured values are:


- Contaminated sensor, or sensor outside of medium
- Sensor defective
- Process error (e.g. through control system)

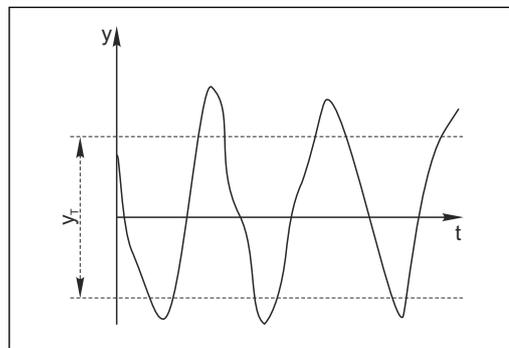

A0027276

1 Normal measuring signal, no alarm

$y$  Measuring signal  
 $y_T$  Minimum signal variation

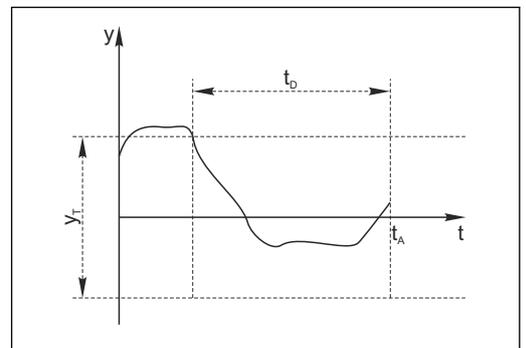

A0027277

2 Stagnating signal, alarm is triggered

$t_D$  Defined time interval  
 $t_A$  Time when the alarm is triggered

**Polarization monitoring (conductive measurement of conductivity only)**

Polarization effects in the boundary layer between the sensor and the measuring solution limit the measuring range of conductive conductivity sensors.

The transmitter can detect and report polarization effects by using a smart signal analysis process.

**United States Pharmacopoeia, USP and European Pharmacopoeia, EP (conductivity only)**

The requirements placed on ultrapure water in the pharmaceutical industry are primarily defined by the American USP and European EP standards.

The transmitter meets the USP/EP requirements for conductivity measuring systems:

- Precise temperature measurement at place of conductivity measurement
- Able to simultaneously display uncompensated conductivity values and temperature
- Display resolution 0.01  $\mu\text{S}/\text{cm}$
- Exact factory calibration of the transmitter with traceable precision resistance values (optional)
- Exact factory calibration of the sensors in accordance with ASTM D 1125-91 or ASTM D 5391-99 (optional)
- Temperature-dependent measured value monitoring according to USP and EP

The limit functions for pharmaceutical water in accordance with USP and EP specifications are implemented in the "Advanced" software package:

- "Water for Injection" (WFI) as per USP <645> and EP
- "Highly Purified Water" (HPW) as per EP
- "Purified Water" (PW) as per EP


The uncompensated conductivity value and the temperature are measured for the USP/EP limit functions. The measured values are compared against the tables defined in the standards. An alarm is triggered if the limit value is exceeded. Furthermore, it is also possible to configure an early warning alarm that signals undesired operating states before they occur.

**Application-optimized calibration models (oxygen)**

The transmitter offers separate functions to enable process-oriented sensor calibration at the zero point or via the slope.

Various calibration models are available for this purpose, ranging from simple slope calibration in water vapor-saturated air to slope calibration by specifying the absolute air pressure and the relative humidity at the place of measurement. The latter model permits in-process calibration both during operation and in sterilization and cleaning phases.

The calibrations and sterilizations are counted separately for the sensor and membrane cap. When a membrane cap is replaced, the corresponding counter can be reset.

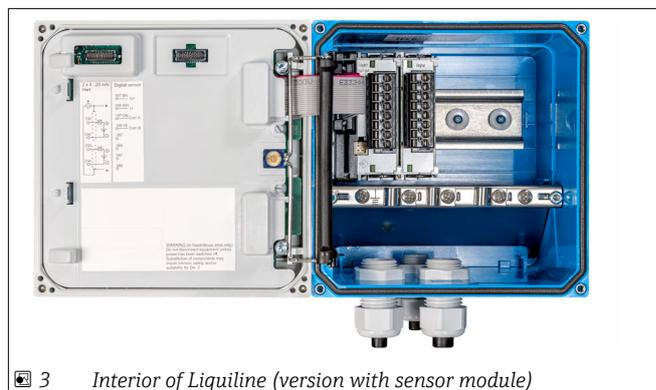**Maintainability****Modular design**


3 Interior of Liquiline (version with sensor module)




4 Plug-in modules

**Sensor monitor ("Advanced version" and "Advanced features" firmware packages only)**

The sensor monitor is located in the DIAG menu. Important sensor data, including warning and alarm limits, are visualized graphically or numerically at a glance.

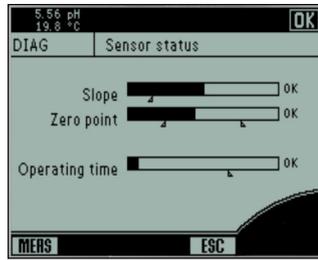


5 Sensor monitor, graphic visualization (example)

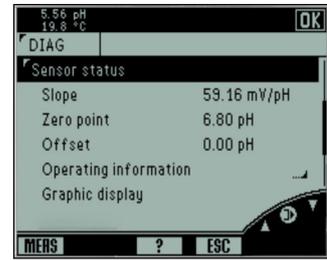


6 Sensor monitor, numeric visualization

**Measuring point monitor (only "Advanced features" firmware package)**

The measuring point monitor is located in the DIAG menu. Important operating data are visualized numerically at a glance.

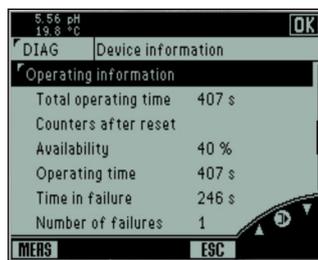

7 Measuring point monitor (example)

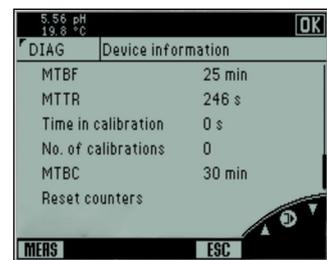

8 Measuring point monitor, continuation

**Safety**

**User administration ("Advanced version" and "Advanced features" firmware packages only)**

The device has a user administration function to prevent unplanned modifications to the measuring point. You must first log in as an Expert to enable the user administration function. Therefore, the first time you log onto the device you are requested to enter a password (the user name "Admin" is then already entered).

In the Advanced version, the user administration function offers two different modes:

**1. Roles**

- There are 3 fixed user roles (Expert, Maintenance, Operator).
- "Experts" always have all levels of authorization. "Operator" is the role with the lowest level of authorization.
- Each role has its own password, which can be modified.
- You cannot create other user roles.

**2. User accounts**

- You can create and manage a maximum of 15 user accounts.
- You may only manage accounts if you are logged on as an "Expert".
- In each user account, you define the user name and the associated password and assign the new user one of the 3 user roles (Operator, Maintenance, Expert).
- More than one user account can have the "Expert" role.

**IT security**

Our warranty is valid only if the device is installed and used as described in the Operating Instructions. The device is equipped with security mechanisms to protect it against any inadvertent changes to the settings.

IT security measures, which provide additional protection for the device and associated data transfer, must be implemented by the operators themselves in line with their security standards.

## Input

**Measured variables** → Documentation of the connected sensor

**Measuring ranges** → Documentation of the connected sensor

## Binary input Memosens



pH/ORP, conductivity, oxygen

<b>Cable specification</b>	CYK10, CYK20 with Memosens	Max. cable length 100 m (330 ft)
	Fixed cable with Memosens (CLS50D, CLS54D)	Max. cable length 100 m (330 ft)

<b>Ex specification</b>	Intrinsically safe sensor circuit with type of protection: Ex ia IIC <sup>1)</sup> or Ex ic IIC <sup>2)</sup> or Ex ib IIC <sup>3)</sup> or 1Ex ib IIC <sup>4)</sup>	
	Max. output voltage $U_o$	5.04 V
	Max. output current $I_o$	80 mA
	Max. output power $P_o$	112 mW

- 1) CM42-\*E\*\*\*\*\*, CM42-\*J\*\*\*\*\*, CM42-\*J\*\*\*\*\*
- 2) CM42-\*V\*\*\*\*\*, CM42-\*F\*\*\*\*\*
- 3) CM42-\*U\*\*\*\*\*
- 4) CM42-\*K\*\*\*\*\*

- ▶ CM42-\*V\*\*00\*\*\*\*\* with the identification marking II 3G Ex nA[ic] IIC T6 Gc are suitable for the connection of Memosens measuring cables CYK10-G\*\*\* with a maximum cable length of 100 m. The sensors connected to the cable must bear at least one of the following identification markings: II 3G Ex ic Tx Gc (Zone 2), II 2G Ex ib Tx Gb (Zone 1), or II 1G Ex ia Tx Ga (Zone 0). The measuring cable and sensor may only ever be operated in connection with CM42-\*V in explosion protection Zone 2.
- ▶ Only sensors that may be arranged in Zone 2 may be connected to CM42-\*F\*\*00\*\*\*\*\* with the identification marking II 3D tc [ic IIC Gc] IIIC T85°C Dc with an "ic"-type Memosens cable (or better); here, the CM42 is arranged in Zone 22.

## Analog input pH/ORP

<b>Cable specification</b>	Without SCS	Max. cable length 50 m (160 ft)
	With SCS	Max. cable length 20 m (65 ft)

**Temperature sensors**

- Pt100
- Pt1000
- NTC 30K

**Ex specification**

Intrinsically safe sensor circuit with type of protection: Ex ia IIC <sup>1)</sup> or Ex ic IIC <sup>2)</sup> or 1Ex ib IIC <sup>3)</sup>		
	<b>Glass</b>	<b>ISFET</b>
Max. output voltage U <sub>o</sub>	10.08 V	10.08 V
Max. output current I <sub>o</sub>	4.1 mA	50.7 mA
Max. output power P <sub>o</sub>	10.2 mW	128 mW
Max. external inductance L <sub>o</sub>	1 mH	1 mH
Max. external capacitance C <sub>o</sub>	250 nF	250 nF
Connection class according to NE116 <sup>4)</sup>	SensISCO1X	-

- 1) CM42-\*E\*\*\*\*\*, CM42-\*I\*\*\*\*\*
- 2) CM42-\*V\*\*\*\*\*, CM42-\*F\*\*\*\*\*
- 3) CM42-\*K\*\*\*\*\*
- 4) CM42-\*E\*\*\*\*\*, CM42-\*F\*\*\*\*\*



When pH/ORP glass electrodes are connected to terminals 317, 318, 320, 111, 112 and 113, the device corresponds to connection class 1 according to NAMUR Recommendation NE116 (SensISCO). Terminals 315 and 316 may not be connected for this classification. The device is labeled SensISCO1X.

**Input impedance** > 10<sup>12</sup> Ω (at rated operating conditions)

**Input leak current** < 10<sup>-13</sup> A (at rated operating conditions)

## Analog input conductivity

**Cable specification**

Conductivity/resistivity, conductive measurement <sup>1)</sup>	
Two-electrode sensor	
10 μS·k to 20 mS·k / 0.1 MΩ/k to 50 Ω/k	Max. cable length 100 m (330 ft)
5 μS·k to 20 mS·k / 0.2 MΩ/k to 50 Ω/k	Max. cable length 50 m (160 ft)
0.1 μS·k to 20 mS·k / 20 MΩ/k to 50 Ω/k	Max. cable length 15 m (50 ft)
Conductivity, conductive measurement	
Four-electrode sensor	
10 μS·k to 1.5 S·k	Max. cable length 100 m (330 ft)
0.1 μS·k to 20 mS·k	Max. cable length 15 m (50 ft)
Conductivity, inductive measurement <sup>2)</sup>	
	Max. cable length 55 m (180 ft) (CLS50)
	Max. cable length 50 m (160 ft) (CLS54)

- 1) With cable CYK71, CPK9 or fixed cable
- 2) With cable CLK5, CLK6 or fixed cable

**Temperature sensors**

- Pt100
- Pt1000

**Ex specification, sensors with conductive measurement of conductivity**

Intrinsically safe sensor circuit with type of protection: Ex ia IIC <sup>1)</sup> or Ex ic IIC <sup>2)</sup>	
Max. output voltage U <sub>o</sub>	10.08 V
Max. output current I <sub>o</sub>	23 mA
Max. output power P <sub>o</sub>	57 mW
Max. external inductance L <sub>o</sub>	300 µH
Max. external capacitance C <sub>o</sub>	50 nF

- 1) CM42-\*G\*\*\*\*\*, CM42-\*E\*\*\*\*\*, CM42-\*I\*\*\*\*\*  
 2) CM42-\*V\*\*\*\*\*, CM42-\*F\*\*\*\*\*

**Ex specification, sensors with inductive measurement of conductivity**

Intrinsically safe sensor circuit with type of protection: Ex ia IIC <sup>1)</sup> or Ex ic IIC <sup>2)</sup> or Ex ib IIC <sup>3)</sup> or 1Ex ib IIC <sup>4)</sup>	
Max. output voltage U <sub>o</sub>	10.08 V
Max. output current I <sub>o</sub>	64 mA
Max. output power P <sub>o</sub>	128 mW
Max. external inductance L <sub>o</sub>	0.1 mH
Max. external capacitance C <sub>o</sub>	1.8 µF

- 1) CM42-\*G\*\*\*\*\*, CM42-\*E\*\*\*\*\*, CM42-\*I\*\*\*\*\*, CM42-\*J\*\*\*\*\*  
 2) CM42-\*V\*\*\*\*\*, CM42-\*F\*\*\*\*\*  
 3) CM42-\*U\*\*\*\*\*  
 4) CM42-\*K\*\*\*\*\*

## Output

**Output signal****Current output**

Depending on version:

- 1x 4 to 20 mA, passive, potentially isolated from the sensor circuit (Memosens only) <sup>1) 2)</sup>
- 2x 4 to 20 mA, passive, potentially isolated from the sensor circuit (Memosens only) and from one another <sup>1) 2) 3)</sup>

**HART**

Signal encoding	FSK ± 0.5 mA above current signal
Data transmission rate	1200 baud
Load (communication resistor)	250 Ω

**PROFIBUS PA**

Signal encoding	Manchester Coding Bus Powered (MBP), in compliance with IEC 61158-2
Data transmission rate	31.25 kBit/s
Bus termination	External
Connection to PROFIBUS-DP network	Via segment coupler (in non-Ex mode)

- 1) In Memosens potential isolation is implemented in the sensor connector  
 2) In the case of inductive sensors with a Memosens protocol CLS50D and CLS54D, not potentially isolated from the sensor circuit!  
 3) Current output 1 and current output 2 (optional)

**FOUNDATION Fieldbus**

Signal encoding	Manchester Coding Bus Powered (MBP), in compliance with IEC 61158-2
Data transmission rate	31.25 kBit/s
Bus termination	External

**Signal on alarm** Configurable, depending on the version:

- 3.6 to 21.5 mA (4.0 mA fixed in HART Multidrop mode)
- Digital via fieldbus <sup>4)</sup>

**Load** Max. load with a supply voltage of 24 V: 500  $\Omega$   
Max. load with a supply voltage of 30 V: 750  $\Omega$

**Output span** 3.6 to 21.5 mA

**Ex specification, current output**

Intrinsically safe power supply and signal circuits, passive	
Max. input voltage $U_i$	30 V
Max. input current $I_i$	100 mA
Max. input power $P_i$	800 mW (all except TIIS) or 750 mW (TIIS)
Max. internal inductance $L_i$	29 $\mu$ H (output 1) 24 $\mu$ H (output 2)
Max. internal capacitance $C_i$	1.2 nF (output 1) 0.2 nF (output 2)

**Ex specification PROFIBUS and FOUNDATION Fieldbus**

Suitable for use as a field device in a FISCO system according to EN/IEC 60079-27	
Max. input voltage $U_i$	17.5 V
Max. input current $I_i$	380 mA
Max. input power $P_i$	5.32 W
Max. internal inductance $L_i$	< 10 $\mu$ H
Max. internal capacitance $C_i$	< 5 nF

**Protocol-specific data****HART**

Manufacturer ID	11 <sub>h</sub>
Device type	11A0 <sub>h</sub> (CM42-M/N/P), 11A1 <sub>h</sub> (CM42-C/I/K/L), 11A2 <sub>h</sub> (CM42-O)
Device revision	001 <sub>h</sub>
Device description files (DD/DTM)	<a href="http://www.endress.com/hart">www.endress.com/hart</a> Device Integration Manager DIM
Device variables	7 (CM42-M/N/O/P), 3 (CM42-C/I/K/L), predefined device variables, dynamic variables PV, SV, TV, QV
Supported features	PDM DD, AMS DD, DTM, Handheld DDs

4) For version with PROFIBUS PA or FOUNDATION Fieldbus

<b>PROFIBUS PA</b>	Manufacturer ID	11 <sub>h</sub>
	Device type	1565 <sub>h</sub> (CM42-M/N/P), 1566 <sub>h</sub> (CM42-C/I/K/L), 1567 <sub>h</sub> (CM42-O) In the compatibility mode: 1543 <sub>h</sub> (CM42-M/N/P), 1544 <sub>h</sub> (CM42-C/I/K/L), 1545 <sub>h</sub> (CM42-O), 1545 <sub>h</sub> (Profile Identifier, Analyzer PA Devices)
	Profile version	3.02
	GSD files	<a href="http://www.endress.com/profibus">www.endress.com/profibus</a> Device Integration Manager DIM
	Output values	6 AI blocks
	Supported features	<ul style="list-style-type: none"> <li>▪ 1 MSCYO connection (cyclical communication, master class 1 to slave)</li> <li>▪ 1 MSAC1 connection (acyclical communication, master class 1 to slave)</li> <li>▪ 2 MSAC2 connections (acyclical communication, master class 2 to slave)</li> <li>▪ Addressing using DIL switches or software</li> <li>▪ GSD, PDM DD, DTM</li> <li>▪ Status output: Condensed oder Classic</li> </ul>

<b>FOUNDATION Fieldbus</b>	Manufacturer Name	Endress+Hauser
	Model Name	Liquiline_pHORP (CM42-M/N/P) or Liquiline_Cond (CM42-C/I/K/L) or Liquiline_Oxygen (CM42-O)
	Manufacturer ID (hex)	452B48
	Device Type (hex)	10A0 (CM42-M/N/P) or 10A1 (CM42-C/I/K/L) or 10A2 (CM42-O)
	Device Revision (hex)	1 (CM42-O) or 2 (CM42-M/N/P/C/I/K/L)
	Device Class	Link Master
	ITK Version	6.1.1
	Function and other Blocks	1xRB, 6xAI, 2xDI, 1xPID, 2xAALM, 1xISEL, 1xSC, 7xTB

## Current output, passive


<b>Span</b>	3.6 to 21.5 mA
<b>Signal characteristics</b>	Linear, table <sup>5)</sup>
<b>Cable specification</b>	Cable type: shielded cable, Ø 2.5 mm (14 AWG)

5) Table only for "Advanced version" and "Advanced features" firmware

## Power supply

### Supply voltage

Current output / HART:

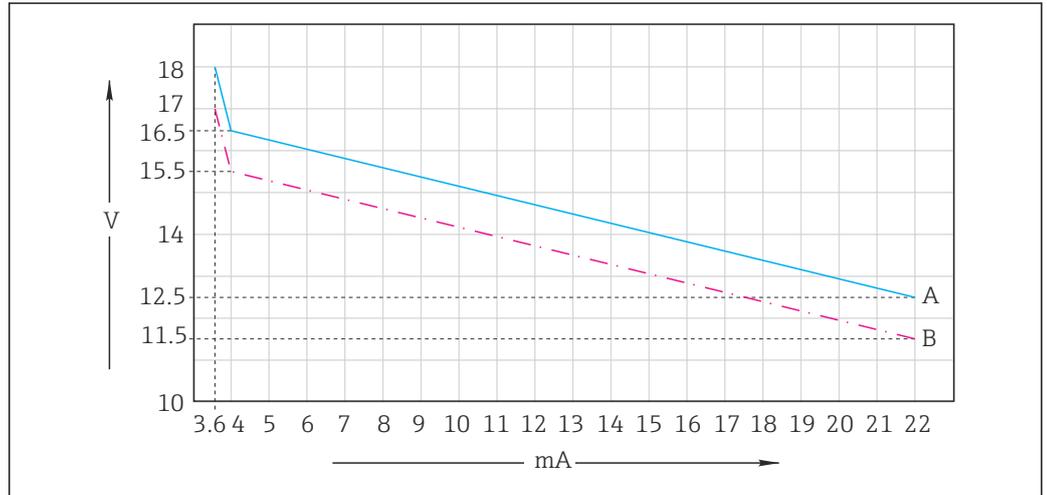

9 Minimum supply voltage at the transmitter depending on the output current

A With HART communication

B Without HART communication

Supply voltage: <sup>1)</sup> max. 30 V DC

Nominal voltage: 24 V DC

- 1) The power supply must meet the relevant safety requirements and be isolated from the mains voltage by double or reinforced insulation.

PROFIBUS/FOUNDATION Fieldbus

Supply voltage

9 to 32 V DC (non-Ex)

9 to 17.5 V DC (Ex, FISCO)

Bus current consumption

22 mA

### Cable specification

#### Qualified cable glands

Cable gland	Clamping area, permitted cable diameter
M16 x 1.5 mm	3 to 6 mm (0.12 to 0.24")
M20 x 1.5 mm	5 to 9 mm (0.20 to 0.35")
M20 x 1.5 mm	6 to 12 mm (0.24 to 0.47")
NPT 3/8"	3 to 6 mm (0.12 to 0.24")
NPT 1/2"	5 to 9 mm (0.20 to 0.35")
NPT 1/2"	6 to 12 mm (0.24 to 0.47")
G3/8	3 to 6 mm (0.12 to 0.24")
G1/2	5 to 9 mm (0.20 to 0.35")
G1/2	9 to 12 mm (0.35 to 0.47")
Dummy plug M16	-
Dummy plug M20	-

#### Cable cross-section

Max. cable cross-section: 2.5 mm<sup>2</sup> (≈14 AWG), GND 4 mm<sup>2</sup> (≈12 AWG)


## Grounding the housing

## Plastic housing

**⚠ WARNING****Electrical voltage at non-grounded cable mounting rail**

No shock protection is provided!

- ▶ Connect the cable mounting rail to the foundation ground using a separate  $\geq 2.5 \text{ mm}^2$  ( $\approx 14$  AWG) functional ground.

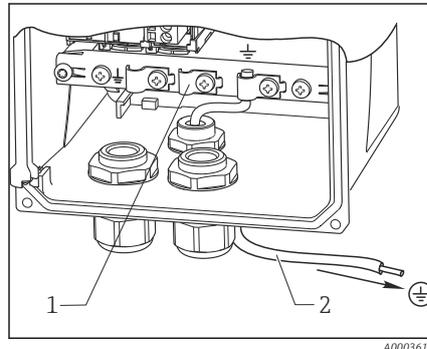

- 1 Cable mounting rail
- 2  $\geq 2.5 \text{ mm}^2$  (14 AWG) functional ground


10 Grounding the housing

## Stainless steel housing

**⚠ WARNING****Electrical voltage at non-grounded housing**

No shock protection is provided!

- ▶ Connect the external ground connection on the housing to the foundation ground using a separate cable (GN/YE) ( $\geq 2.5 \text{ mm}^2$ ,  $\approx 14$  AWG).

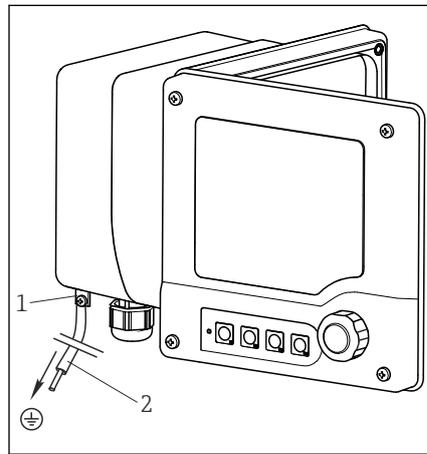

- 1 External ground connection
- 2  $\geq 2.5 \text{ mm}^2$  ( $\approx 14$  AWG) cable (GN/YE)


11 Grounding the housing

**Power supply and signal circuit**


**4 to 20 mA**

- ▶ Connect the transmitter with a shielded two-wire cable.
  - ↳ The type of shield connection depends on the anticipated interference influence. To suppress electrical fields, it suffices to ground the shield on one side. If you also want to suppress interference from an alternating magnetic field, you must ground the shield on both sides.

**i** The second current output can be ordered as an optional extra (Product Configurator on [www.endress.com/cm42](http://www.endress.com/cm42)).

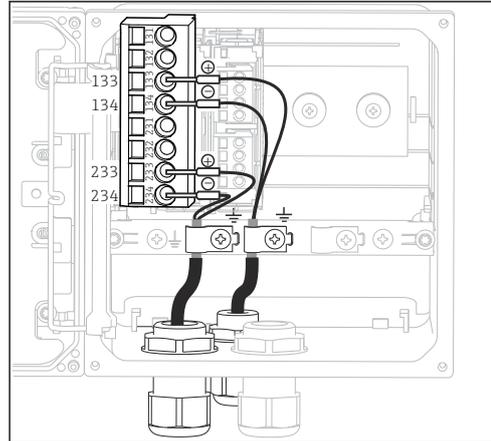

**12** In-device view (CPU module)

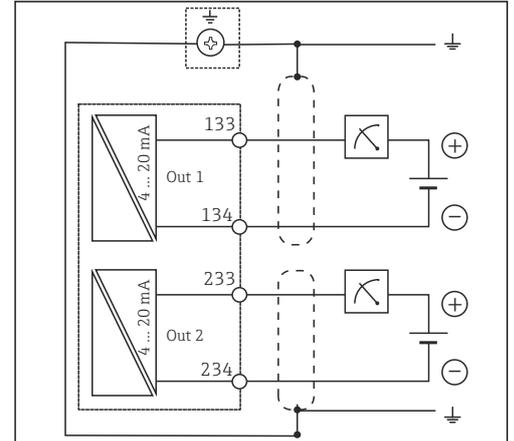


**13** Wiring diagram

The figures show the version with the shield grounded at both sides to suppress interference from an alternating magnetic field.


**4 to 20 mA / HART**

You must use a two-wire cable grounded on both sides to ensure secure communication via the HART protocol and to comply with NAMUR NE 21 specifications.

- ▶ Connect the transmitter with a two-wire cable grounded at both sides.

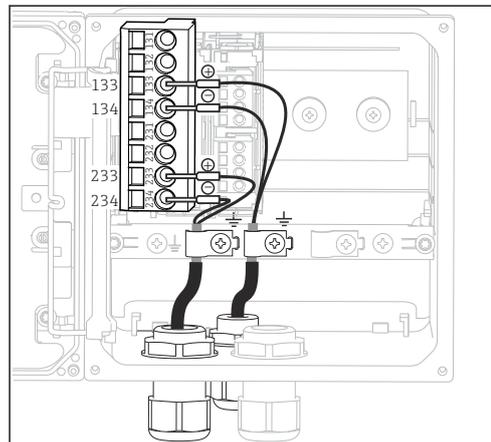

**14** In-device view (CPU module)

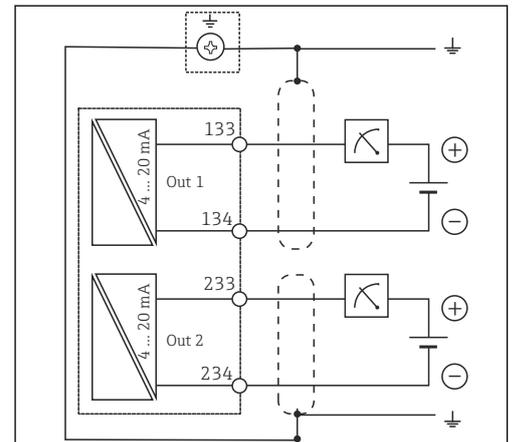

**15** Wiring diagram

**i** Power is only supplied to the device via current output 1, not via current output 2.


**PROFIBUS PA and FOUNDATION Fieldbus**

Use a fieldbus cable grounded on both sides (device **and** PCS).


There are various ways to establish the connection:

1. Two-wire cable grounded on both sides, "hard grounding" (generally to be preferred over "capacitive ground connection")


2. If there is a risk of large potential equalization currents:  
Shielded two-wire cable, "Capacitive ground connection"  
(shield grounded at the device via capacitor, "C-module" accessory required)  
**Not for use in the hazardous area!**
3. Using the fieldbus connection socket (accessories)

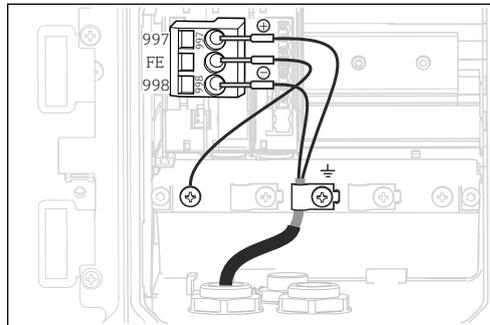*"Hard grounding"*


16 In-device view (CPU module)

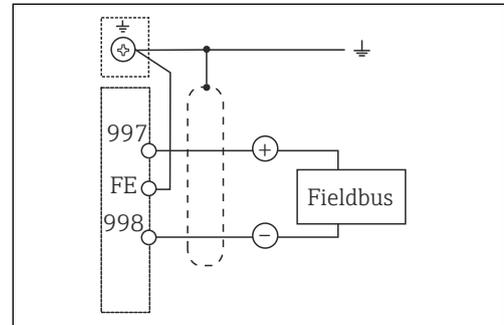


17 Wiring diagram

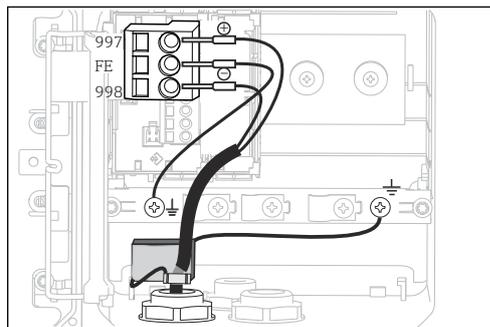*"Capacitive ground connection" with the C-module*


18 In-device view (CPU module)

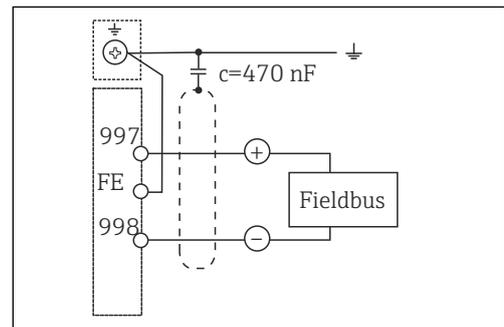

19 Wiring diagram

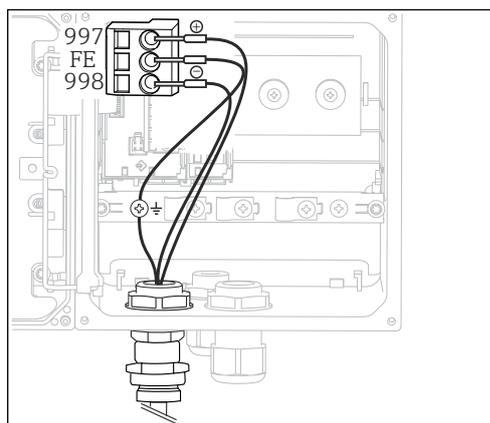*"Fieldbus connection socket"*

20 In-device view (CPU module)

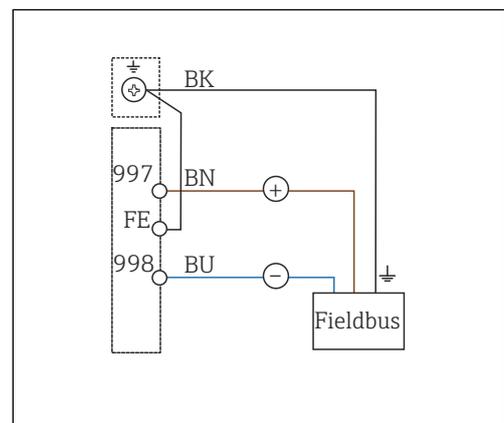

21 Wiring diagram

Sensor connection

**NOTICE**

**No shield against electrical and magnetic interference**

Interference can lead to incorrect measurement results!

- ▶ Connect shielded connections or terminals to the functional ground ( $\ominus$ ) (there is no protective ground on the plastic housing ( $\oplus$ )).
- ▶ Keep magnetic interference away from the sensor, as inductive conductivity sensors use magnetic fields.


Explanation of abbreviations used in the following graphics:

Abbreviation	Meaning
pH	pH signal
Ref	Signal from reference electrode
Src	Source
Drn	Drain
PM	Potential matching
U <sub>+</sub>	Power supply of digital sensor
U <sub>-</sub>	
Com A	Communication signals of digital sensor
Com B	
ϑ	Signal of temperature sensor
d.n.c.	do not connect


**Memosens sensors**



**Connection via Memosens cable CYK10**

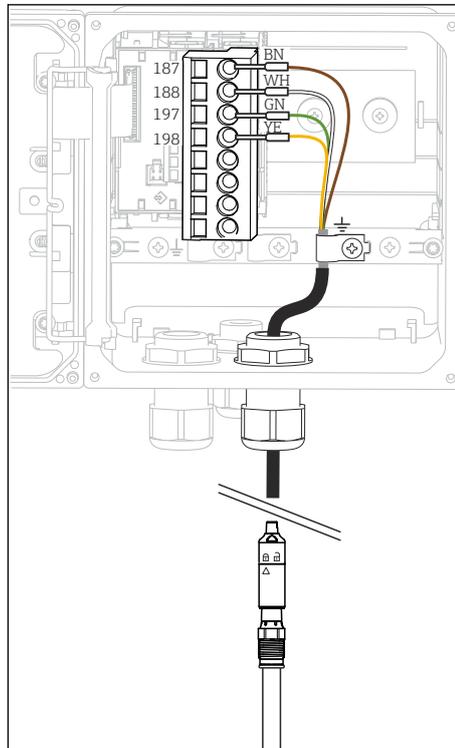


22 In-device view (sensor module)

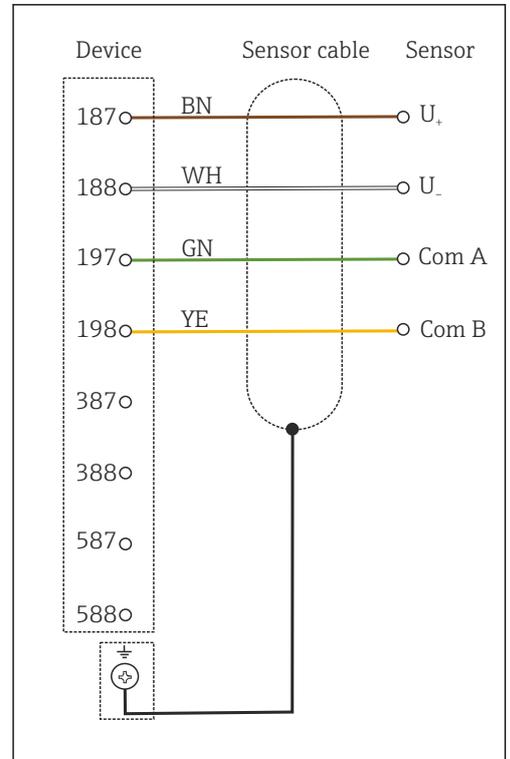


23 Wiring diagram



Connection via sensor fixed cable

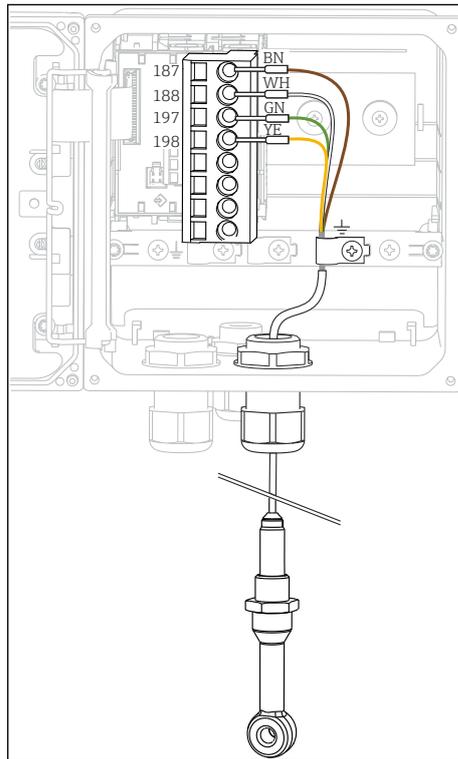

24 In-device view (sensor module)

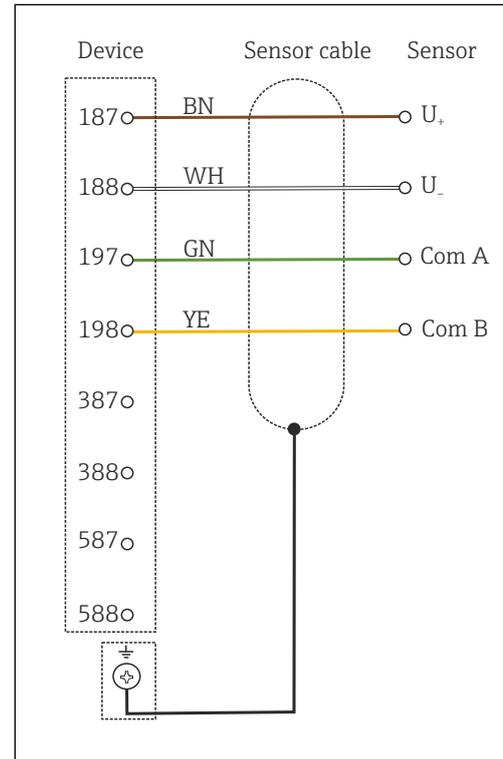


25 Wiring diagram

CLS50D: from serial numbers J3xxxx05LI0


CLS54D: from serial numbers H9xxxx05LI1

Analog pH/ORP sensors

Glass electrodes, with PML (symmetrical)

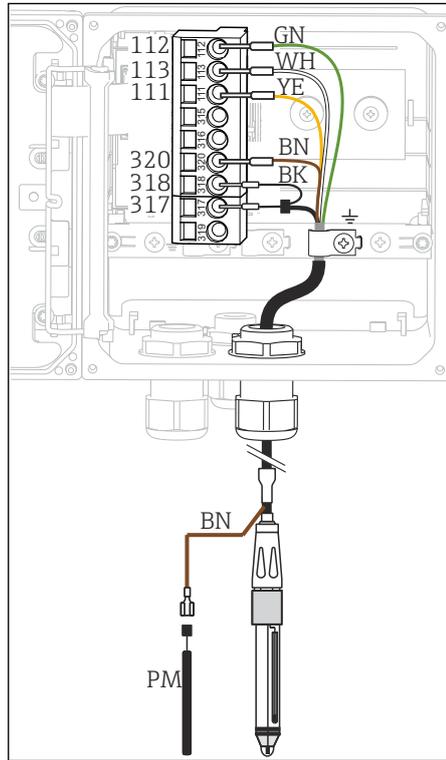


26 In-device view (sensor module)

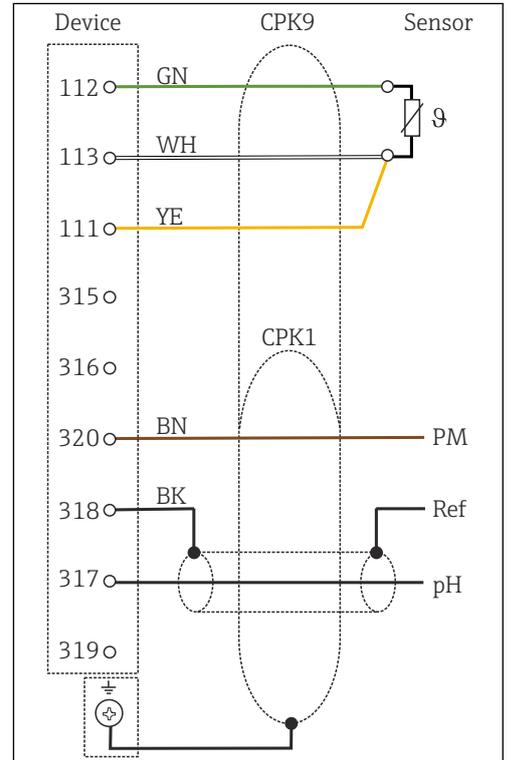


27 Wiring diagram

Glass electrodes, without PML (asymmetrical)

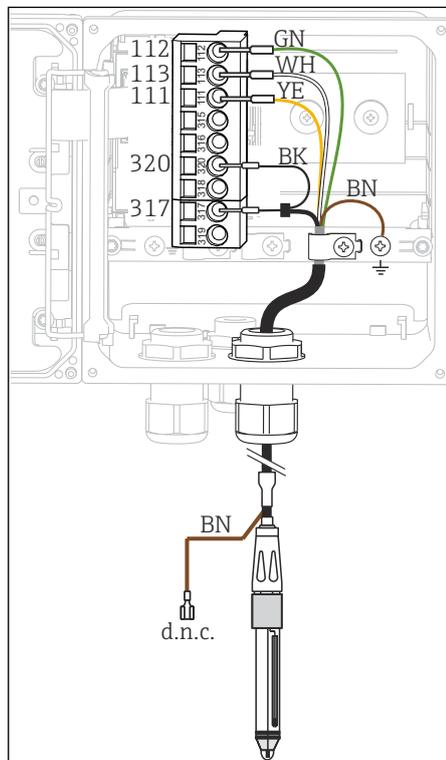


28 In-device view (sensor module)

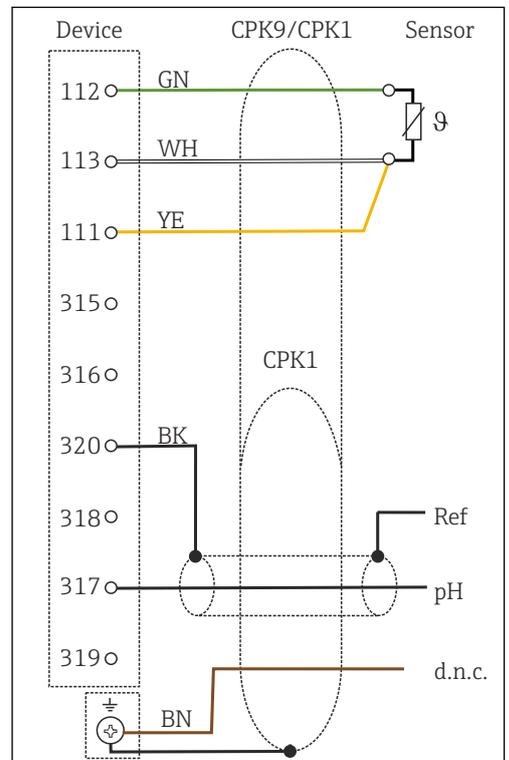


29 Wiring diagram

**ISFET sensors, with PML (symmetrical)**

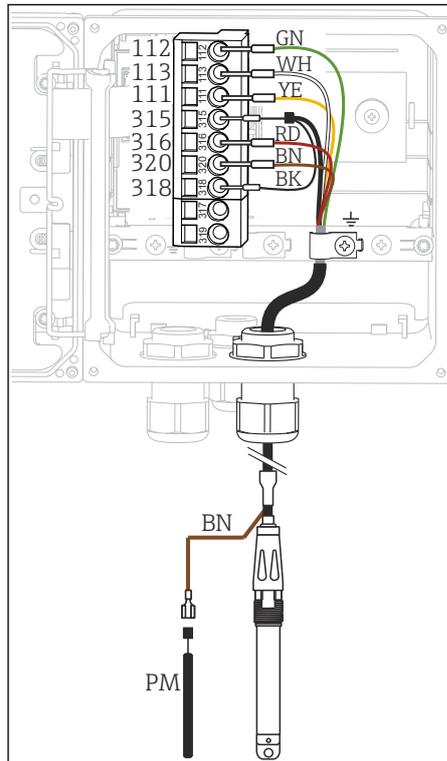


30 In-device view (sensor module)

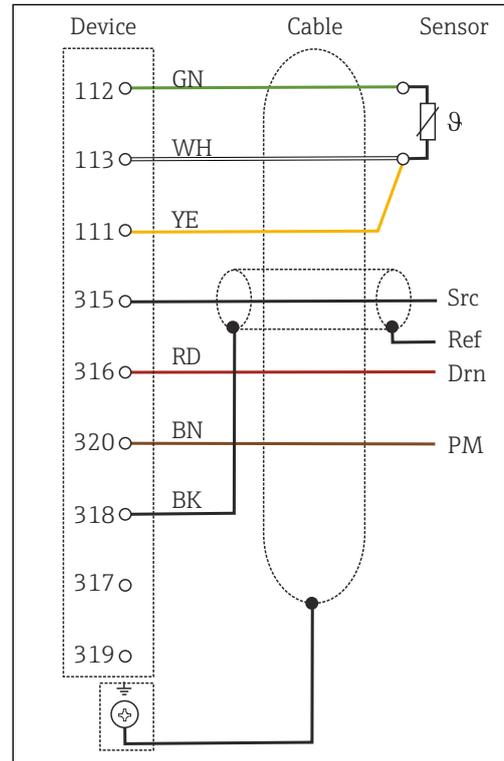


31 Wiring diagram

**ISFET sensors, without PML (asymmetrical)**

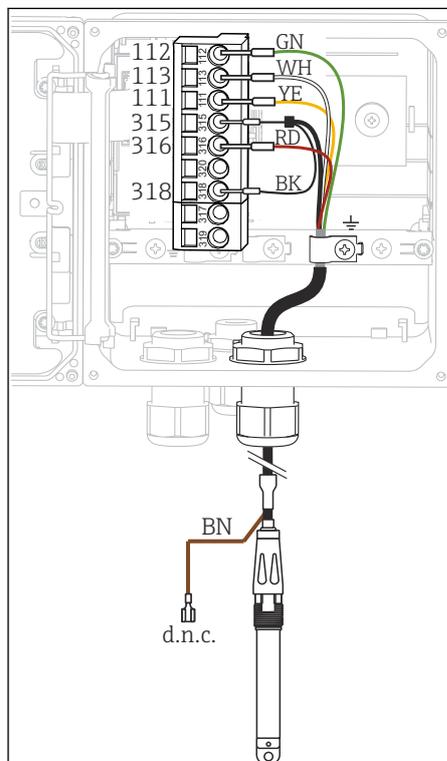

32 In-device view (sensor module)

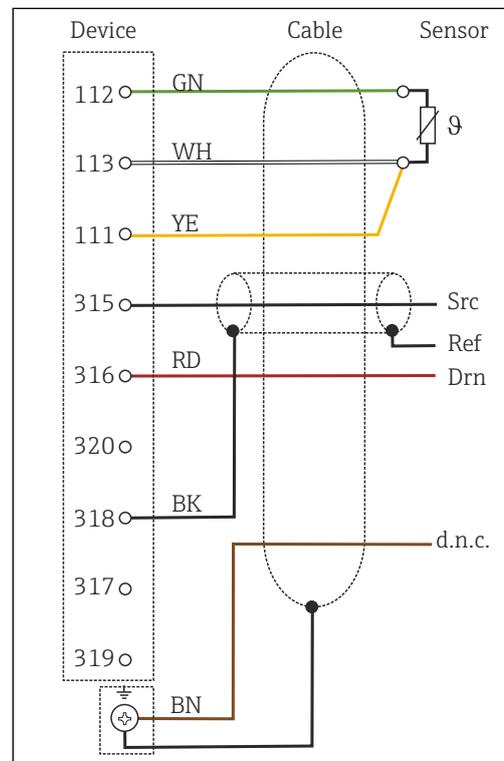


33 Wiring diagram

**pH enamel electrodes**

**With PML (symmetrical)**


Pfaunder electrode, absolute  
Type 03 / type 04

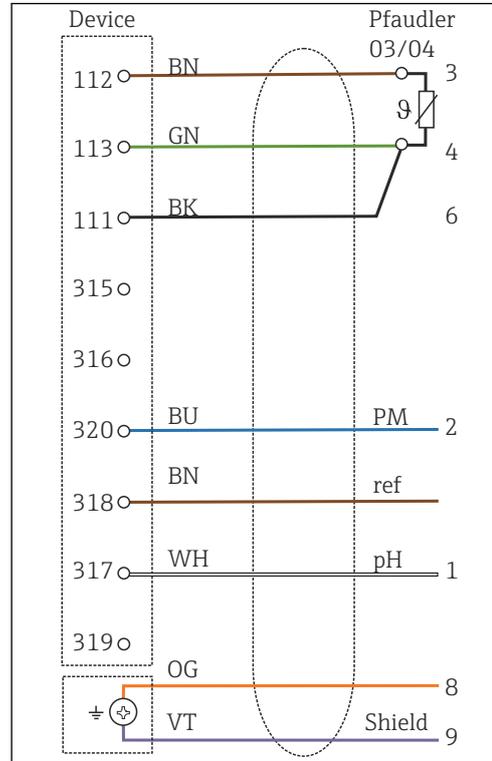

34 Wiring diagram

**With PML (symmetrical)**


Pfaunder electrode, relative  
Type 18 / type 40

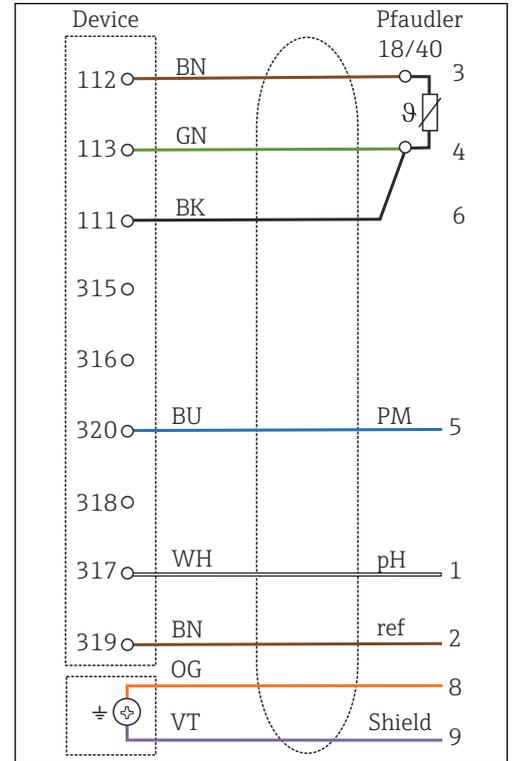

35 Wiring diagram

**With PML (symmetrical)**


pH-Reiner

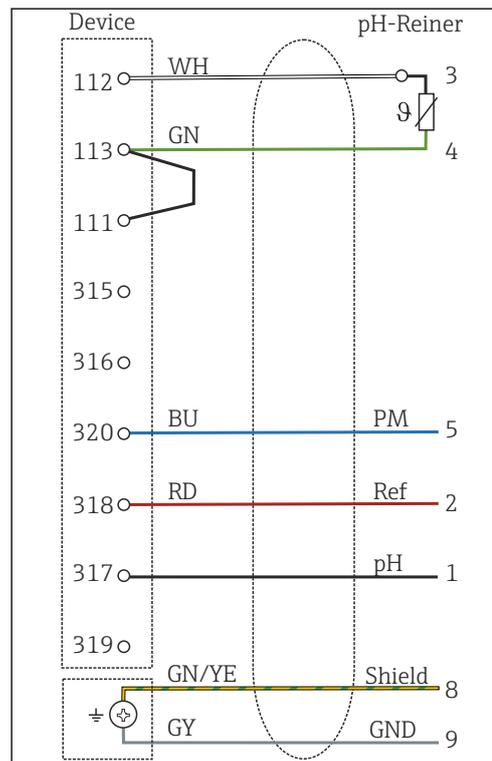

36 Wiring diagram


**Without PML (asymmetrical)**

Pfaunder electrode, absolute  
Type 03 / type 04

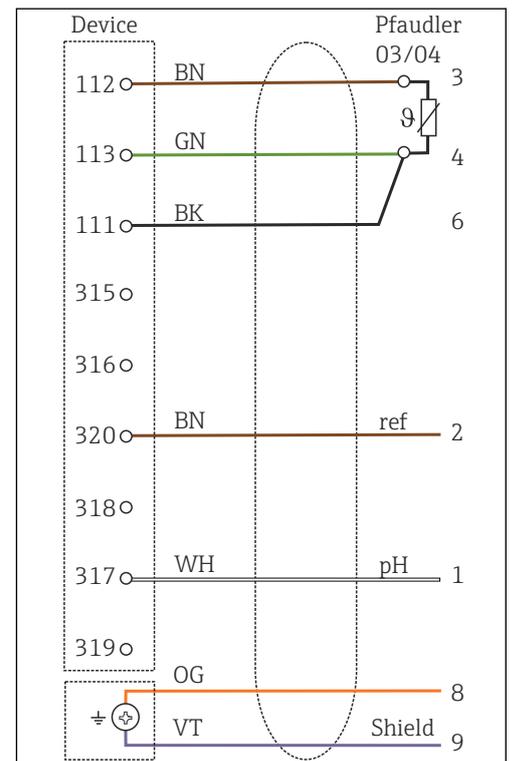


37 Wiring diagram

**Single electrodes (e.g. CPS64 glass or antimony), without PML (asymmetrical)**

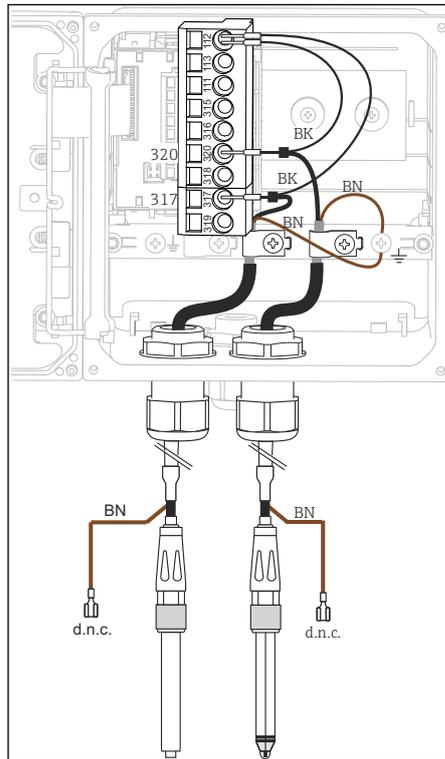


38 In-device view (sensor module)

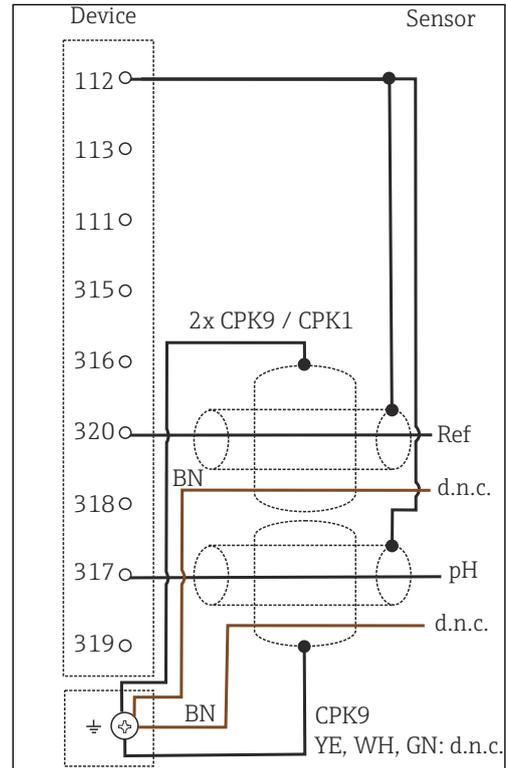

39 Wiring diagram

**Glass electrode and ORP sensor for rH measurement**

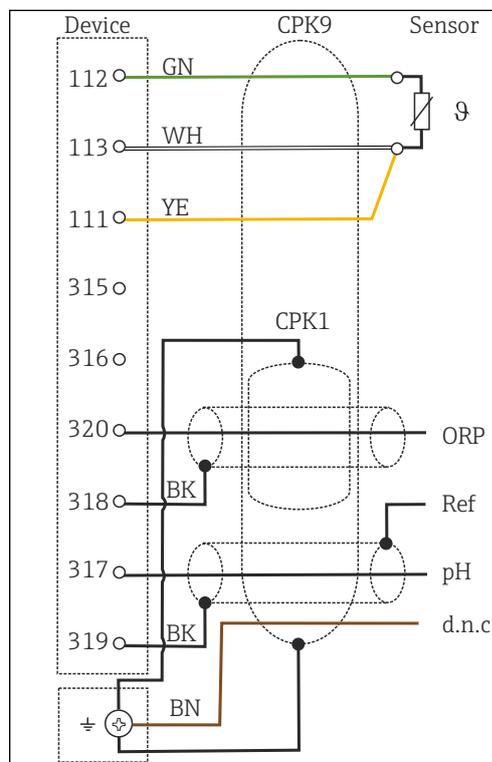


40 Wiring diagram


**i** For rH measurement, connect a pH sensor (e.g. CPS11 with CPK9 sensor cable) **and** an ORP sensor (e.g. CPS12 with CPK1 sensor cable).

**Analog conductivity sensors**

**Sensors with conductive measurement of conductivity, two-electrode sensors**

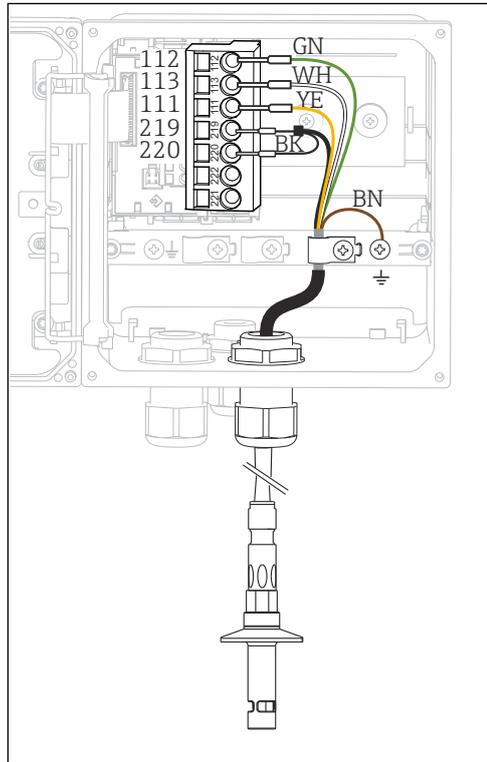


41 In-device view (sensor module)

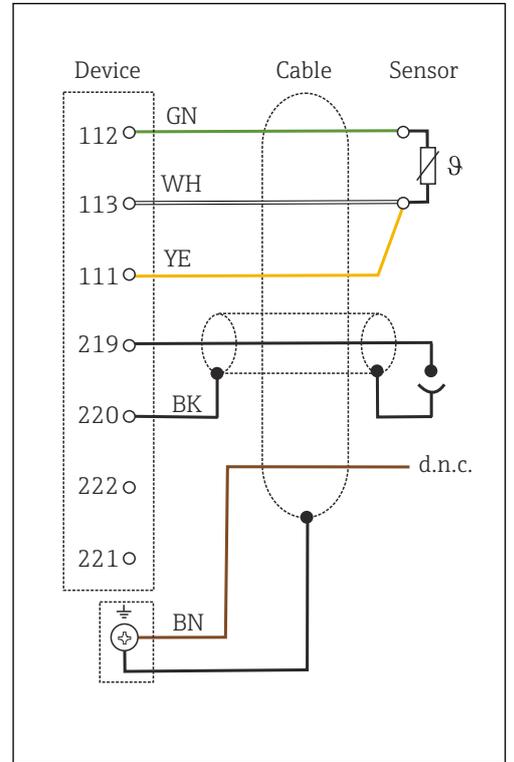


42 Wiring diagram

**Sensors with conductive measurement of conductivity, four-electrode sensors**

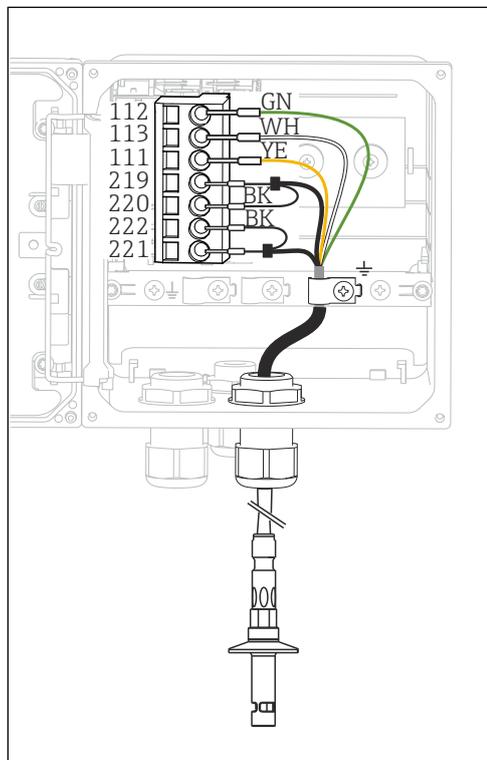


43 In-device view (sensor module)

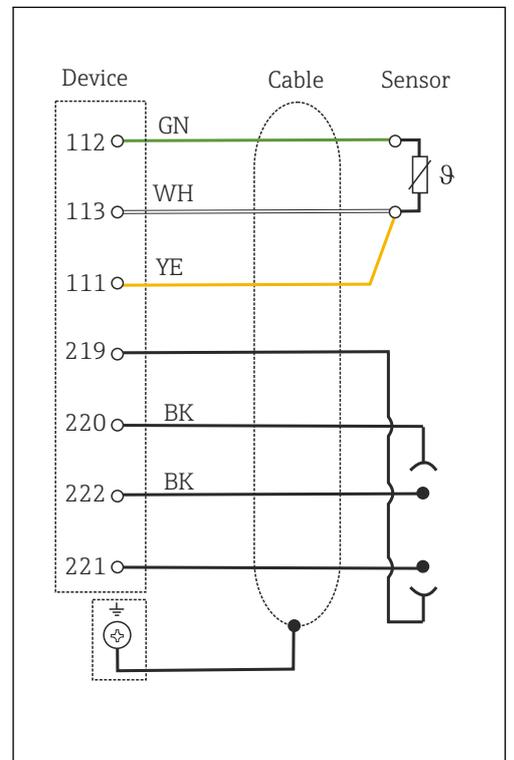


44 Wiring diagram


**Sensors with inductive measurement of conductivity**

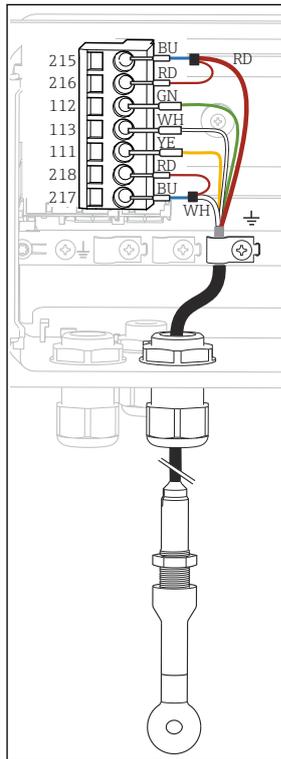

45 In-device view (sensor module)

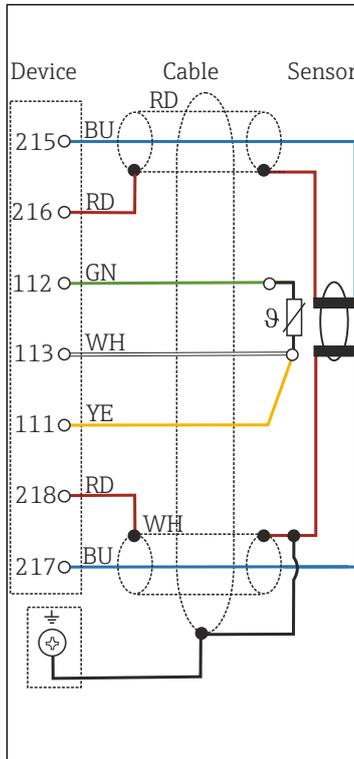

46 Wiring diagram CLS50

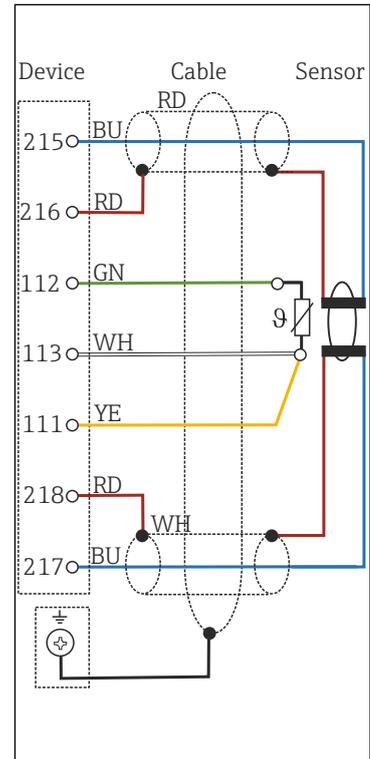

47 Wiring diagram CLS54

**Performance characteristics**

**Response time of current output**

$t_{90}$  = max. 500 ms for an increase from 4 to 20 mA

**Maximum measured error Memosens**

Thanks to digital data transmission, the measured value supplied by the sensor is passed on exactly at the sensor input. The accuracy depends solely on the connected sensor and the quality of its adjustment.

**Tolerance, current outputs**

Additionally 25  $\mu$ A

**Repeatability**

→ Documentation of the connected sensor

**Temperature compensation, conductivity**

Types of compensation	Range
None	$\alpha$ = 0.00 to 20.00 %·K <sup>-1</sup>
Linear NaCl as per IEC 746-3	0 to 100 °C (32 to 212 °F)
Natural water as per IEC 7888	0 to 35 °C (32 to 95 °F)
Ultrapure water NaCl	0 to 100 °C (32 to 212 °F)
Ultrapure water HCl (also for NH <sub>3</sub> )	0 to 60 °C (32 to 140 °F)
4 user-definable tables <sup>1)</sup>	

1) With the "Advanced version" or "Advanced features" firmware package


**Temperature adjustment**

Temperature offset	-5 to +5 °C (23 to 41 °F)
--------------------	---------------------------

# Installation

**Installation conditions**

**Mounting plate**

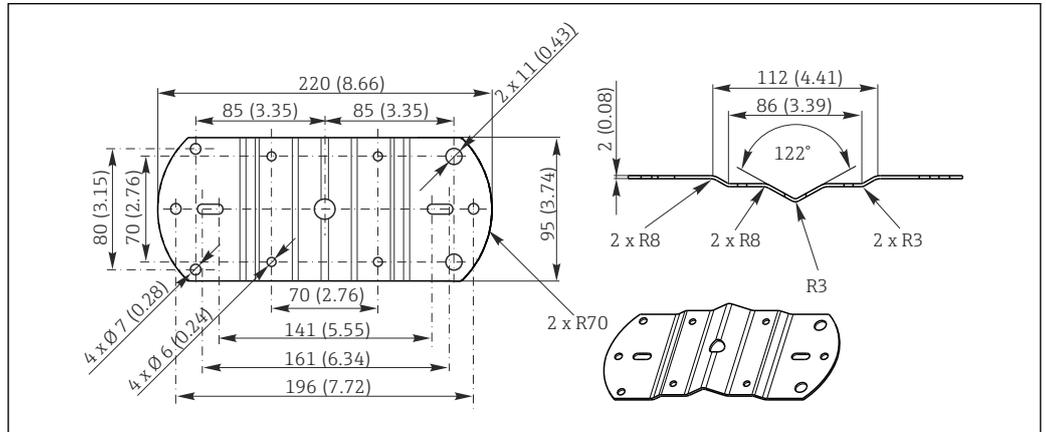

A0032497

48 Dimensions in mm (inch)

**Weather protection cover**


**NOTICE**

**Effect of climatic conditions: rain, snow, direct sunlight**

Device damage to total device failure is possible!

- ▶ When installing outside, always use the weather protection cover. (→ 38)


*For transmitter with plastic housing*

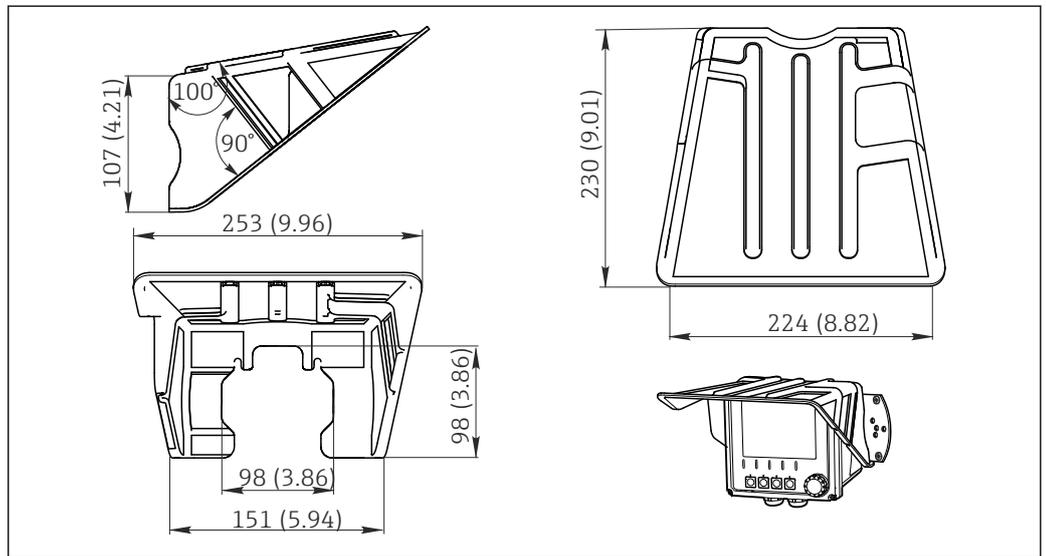

A0032495

49 Dimensions in mm (inch)

For transmitter with stainless steel housing

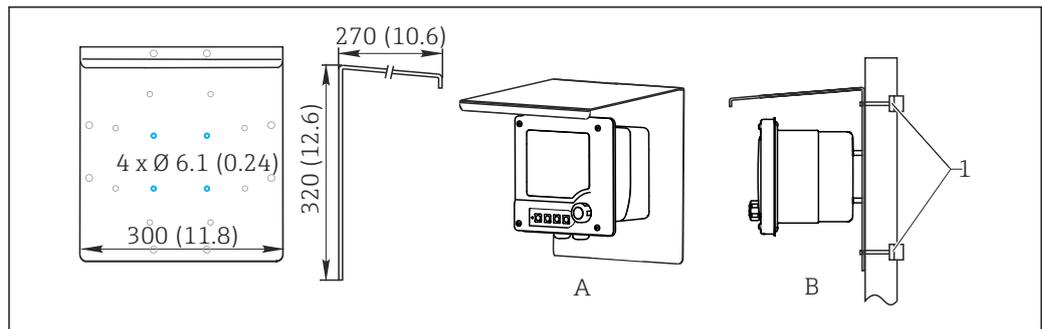


A0032496

50 Dimensions in mm (inch)

Installation in hazardous areas

CM42-\*E/I/J/K

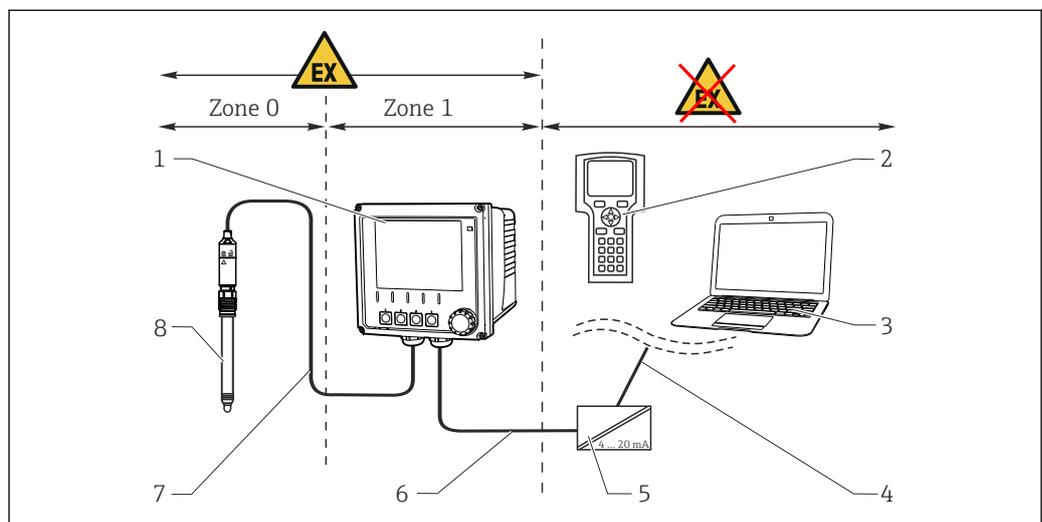


A0032486

51 Installation in hazardous area Ex ib (ia Ga)

- |   |  |
|---|--|
| 1 Transmitter                                   | 5 Active barrier, e.g. RN221                   |
| 2 HART handheld terminal                        | 6 Supply and signal circuit Ex ib (4 to 20 mA) |
| 3 FieldCare via PROFIBUS/FOUNDATION Fieldbus    | 7 Intrinsically safe sensor circuit Ex ia      |
| 4 Signal line HART/PROFIBUS/FOUNDATION Fieldbus | 8 Hazardous area version of sensor             |

CM42-\*F

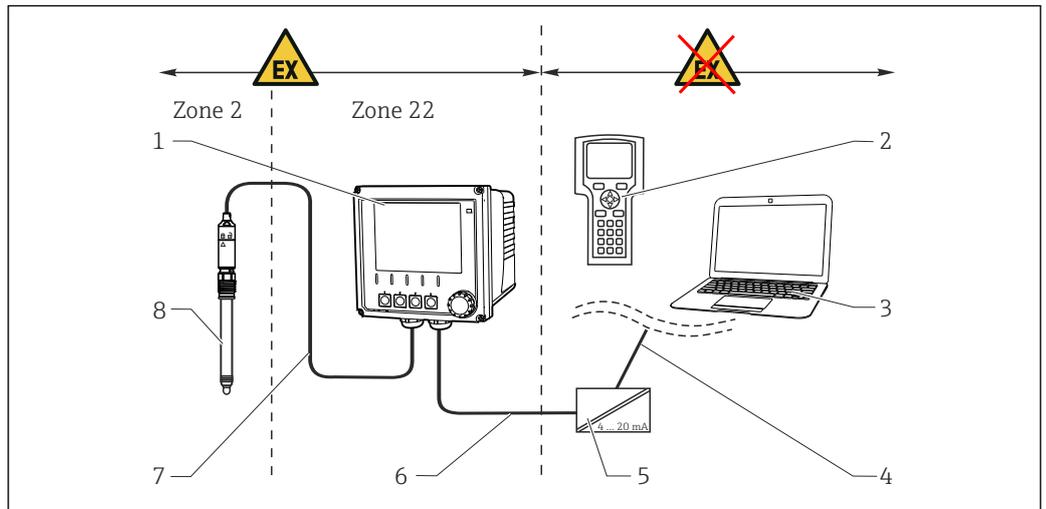


A0032487

52 Installation in hazardous area Ex tc (ic)

- |   |  |
|---|--|
| 1 Transmitter                                   | 5 Active barrier, e.g. RN221             |
| 2 HART handheld terminal                        | 6 Supply and signal circuit (4 to 20 mA) |
| 3 FieldCare via PROFIBUS/FOUNDATION Fieldbus    | 7 Intrinsically safe sensor circuit      |
| 4 Signal line HART/PROFIBUS/FOUNDATION Fieldbus | 8 Hazardous area version of sensor       |

CM42-\*V

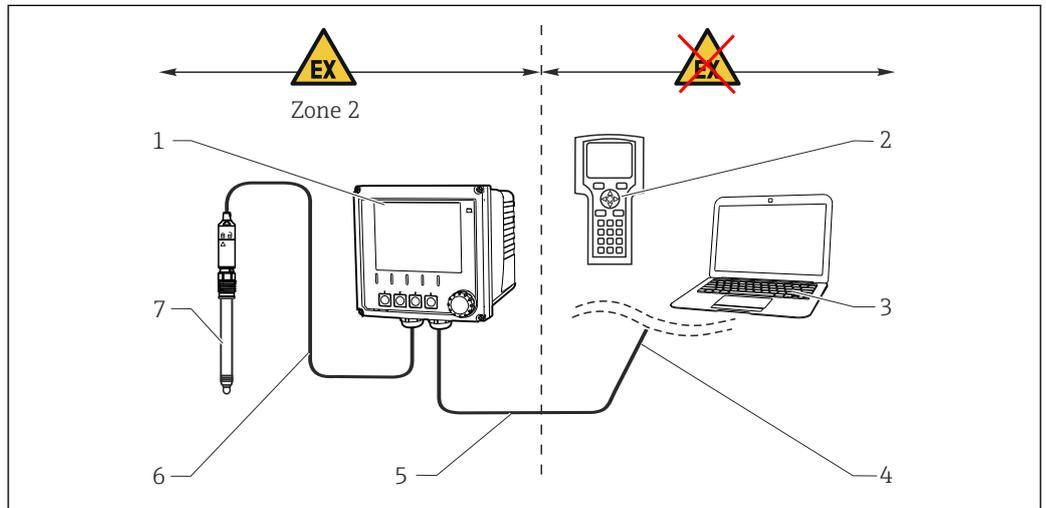


A0032488

53 Installation in hazardous area Ex nA (ic)

- |   |  |
|---|--|
| 1 Transmitter                                   | 5 Supply and signal circuit Ex nA (4 to 20 mA) |
| 2 HART handheld terminal                        | 6 Intrinsically safe sensor circuit Ex ic      |
| 3 FieldCare via PROFIBUS/FOUNDATION Fieldbus    | 7 Hazardous area version of sensor             |
| 4 Signal line HART/PROFIBUS/FOUNDATION Fieldbus |  |

CM42-\*P/S

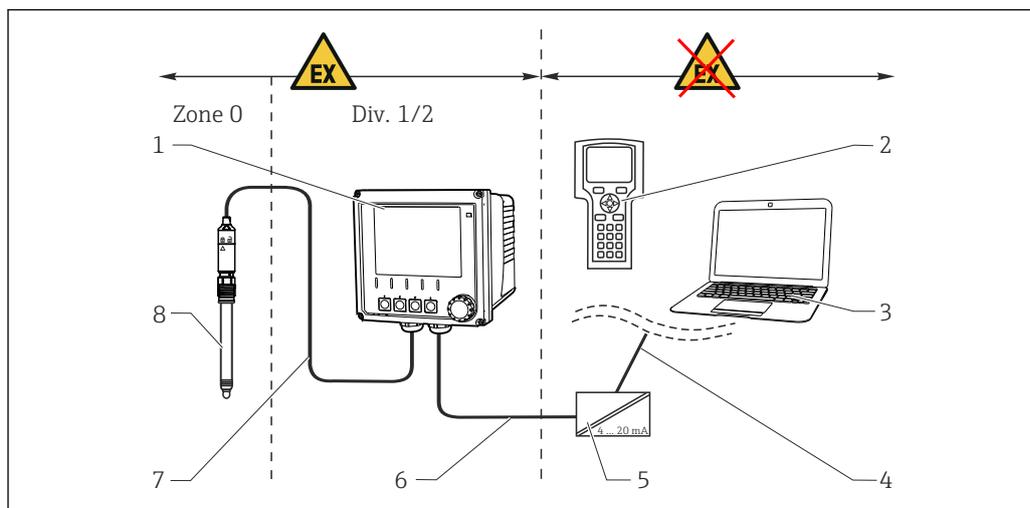


A0032489

54 Installation in hazardous area FM/CSA

- |   |  |
|---|--|
| 1 Transmitter                                   | 5 Active barrier, e.g. RN221             |
| 2 HART handheld terminal                        | 6 Supply and signal circuit (4 to 20 mA) |
| 3 FieldCare via PROFIBUS/FOUNDATION Fieldbus    | 7 Intrinsically safe sensor circuit      |
| 4 Signal line HART/PROFIBUS/FOUNDATION Fieldbus | 8 Hazardous area version of sensor       |

CM42-\*U



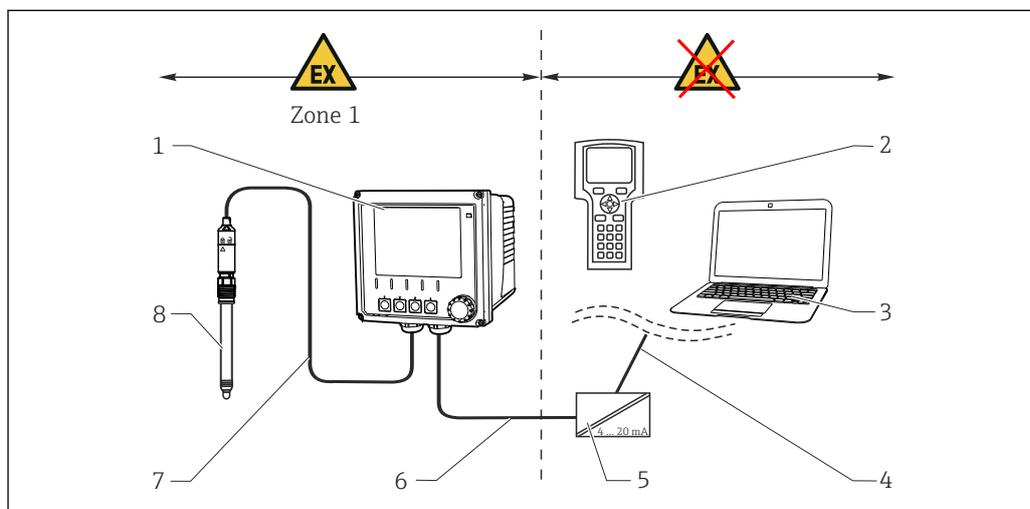


A0032491

55 Installation in hazardous area JPN

- |                          |  |
|--------------------------|--|
| 1 Transmitter            | 5 Active barrier, e.g. RN221             |
| 2 HART handheld terminal | 6 Supply and signal circuit (4 to 20 mA) |
| 3 FieldCare              | 7 Intrinsically safe sensor circuit      |
| 4 HART signal line       | 8 Hazardous area version of sensor       |

**Installation options**

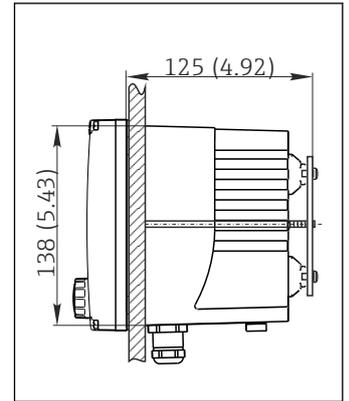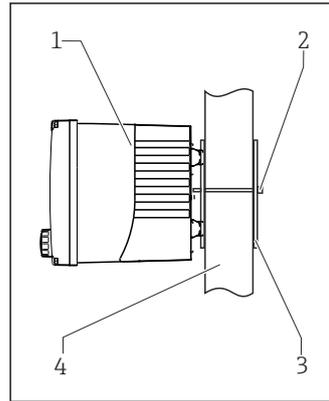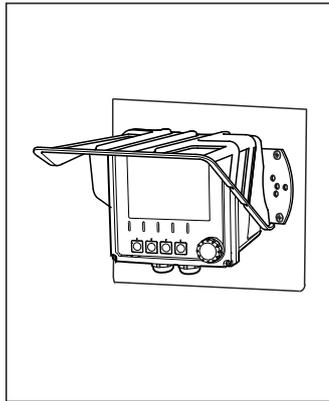

56 Wall mounting  
optional weather protection cover

57 Post mounting  
1 Liquiline  
2, 3 Mounting plate (1x accessory)  
4 Pipe/post (circular/square)

58 Panel mounting

		Wall mounting	Mounting on a pipe	Panel mounting
	<b>Plastic housing</b>			
	Without weather protection cover	Mounting plate: standard	Mounting kit: 51518263	Installation kit: 51518173
	With weather protection cover	Protective cover: 51517382	Mounting kit: 51518263 Protective cover: 51517382	
	<b>Stainless steel housing</b>			
	Without weather protection cover	Mounting plate: standard	Mounting kit: 51518286	Installation kit: 51518284
	With weather protection cover	Protective cover: CYY101-A	Protective cover: CYY101-A Circular post attachment: 50062121	

**Environment**

**Ambient temperature**

**Non-Ex version**

-30 to 70 °C (-20 to 160 °F)

**Hazardous area version: ATEX (1)2G, IECEx ib Gb [ia Ga], NEPSI ib Gb [ia Ga], EAC Ex ib Gb [ia Ga]**

-20 to 50 °C (T6)

-20 to 55 °C (T4)

**ATEX II 3D tc [ic], ATEX/NEPSI II 3G Ex nA[ic]**

-10 to 50 °C (T6)

**Hazardous area version: JPN Ex ib [ia Ga] IIC T6 Gb**

-20 to 55 °C (T4)

**Hazardous area version: CSA Class I, II, III, Div. 1&2 or CSA C/US Class I, Div. 1&2**

-20 to 50 °C (0 to 120 °F) (T6)

-20 to 55 °C (0 to 130 °F) (T4)

**Hazardous area version: FM Class I, Div 1&2**

-20 to 50 °C (0 to 120 °F) (T6)

**Storage temperature**

-40 to +80 °C (-40 to 175 °F)


**Humidity**

10 to 95 %, non-condensating

<b>Degree of protection</b>	IP66/67, tightness and corrosion resistance in accordance with NEMA TYPE 4X
<b>Electromagnetic compatibility</b>	According to IEC 61326-1:2012 <ul style="list-style-type: none"> <li>■ Interference immunity: Table 2 (industrial environments)</li> <li>■ Interference emission: Class B (residential environments)</li> </ul>
<b>Degree of contamination</b>	The product is suitable for pollution degree 3 according to EN 61010-1.

## Mechanical construction


**Dimensions** Plastic housing

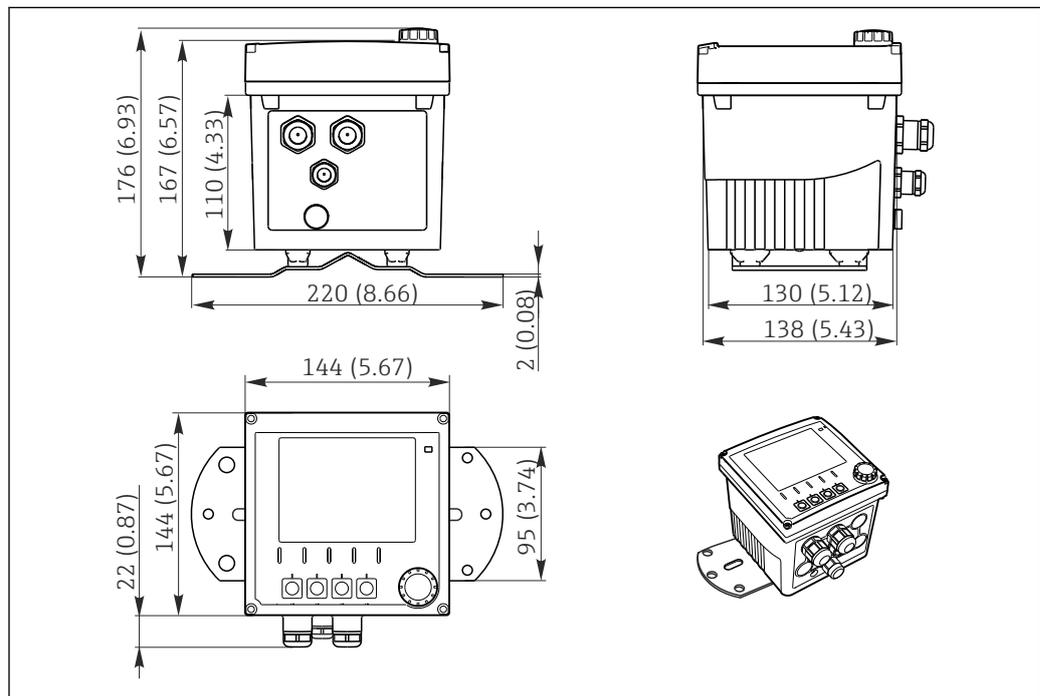

59 Dimensions in mm (inch)

A0032526

**Stainless steel housing**

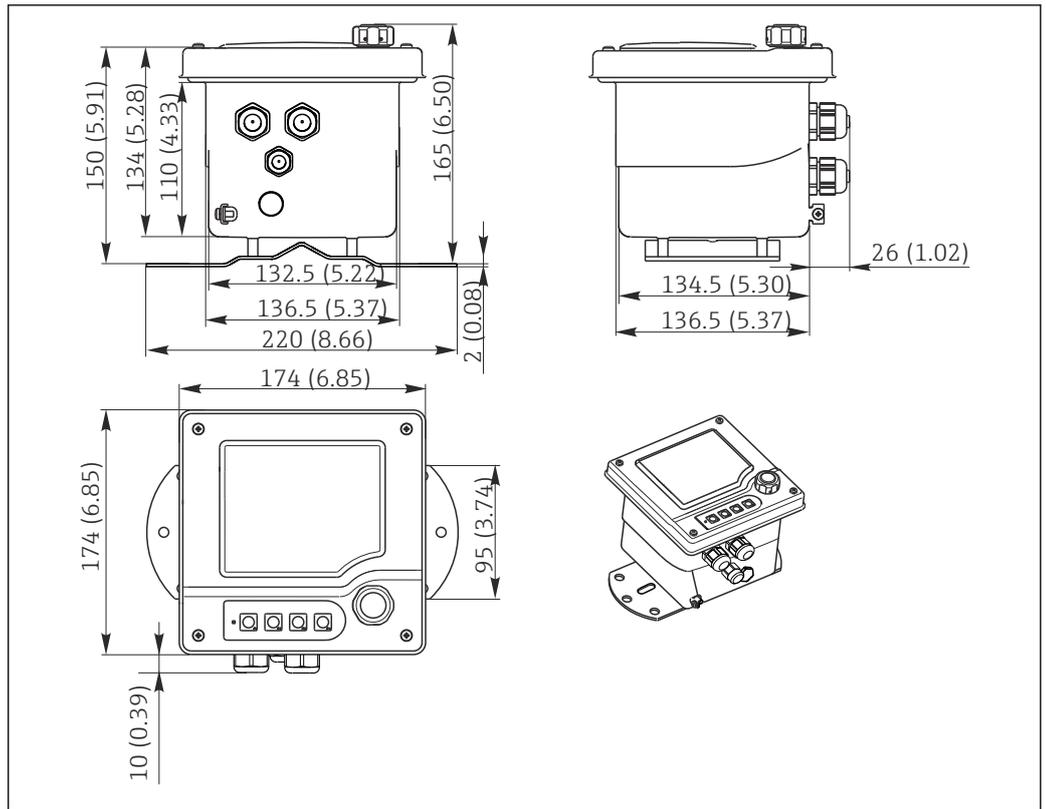

60 Dimensions in mm (inch)

A0032498

**Weight**

**Plastic housing**

1.5 kg (3.3 lbs)

**Stainless steel housing**

2.1 kg (4.6 lbs)

**Materials**

<b>Plastic housing</b>	
Housing	PC-FR (polycarbonate, flame-retarding)
Housing seals	Silicone, foamed, EPDM
<b>Stainless steel housing</b>	
Housing	Stainless steel 1.4301 (AISI 304)
Housing seals	EPDM (ethylene propylene diene rubber)
<b>Plastic and stainless steel housing</b>	
Module housing	PC (polycarbonate)
Soft keys	TPE (thermoplastic elastomers)
Cable mounting rail	Stainless steel 1.4301 (AISI 304)
Display glass	PC-FR (polycarbonate, flame-retarding)
Cable glands	PA (polyamide) V0 as per UL94
Dummy plug M16 and M20	PA (polyamide) V0 as per UL94

## Operability


### Operating concept

The simple and structured operating concept sets new standards:

- Fewer user errors thanks to very easy operation
- Quick configuration using the Navigator
- Intuitive configuration and diagnostics thanks to plain-text display



61 Navigator

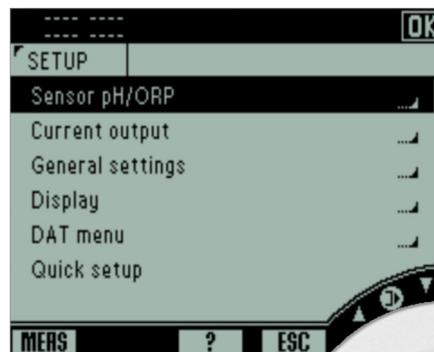

62 Plain-text menu


### Local operation

#### Display

LCD display:

- FSTN technology (FSTN = Foil Super Twisted Nematic)
- Size: 94 x 76 mm (3.7 x 3.0")
- Resolution: 240 x 160 dots

#### Operating elements

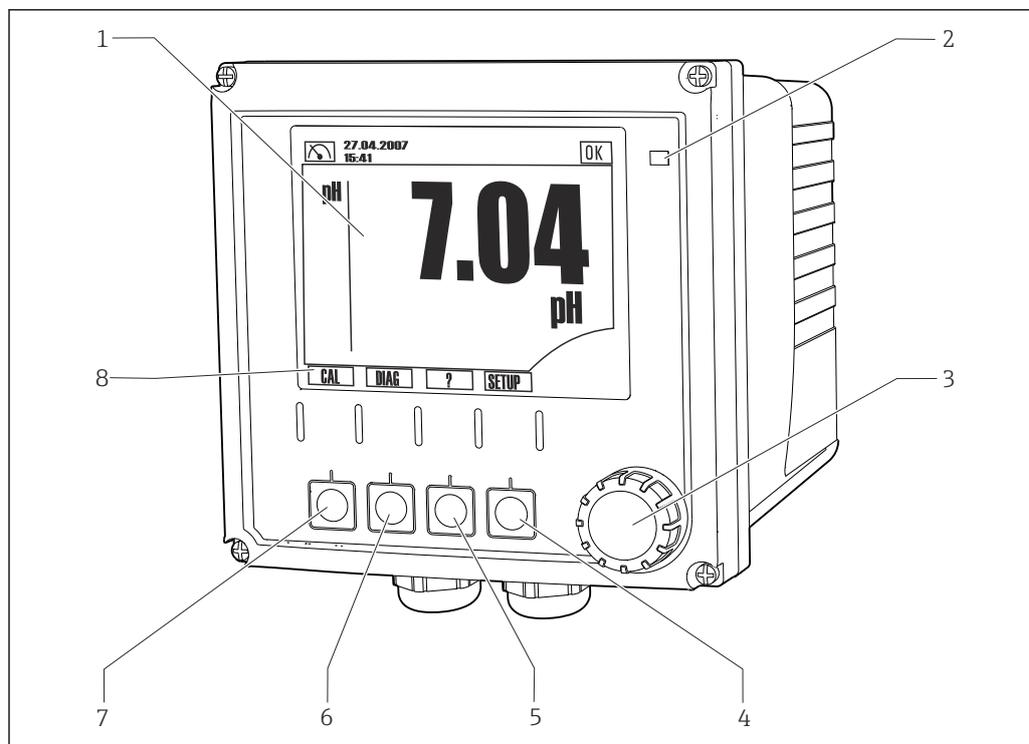

A0032528

63 Overview of operation

- 1 Display, current display: pH measuring mode
- 2 Alarm LED
- 3 Navigator
- 4-7 Soft keys
- 8 Displays the soft key function (menu-dependent)

**Language packages**

The language selected in the product structure is the operating language preset at the factory.


- English (US)
- German
- Chinese (Simplified, PR China)
- Czech
- Dutch
- French
- Italian
- Japanese
- Polish
- Portuguese
- Russian
- Spanish
- Swedish
- Korean

The availability of other languages can be checked via the product structure at [www.endress.com/CM42](http://www.endress.com/CM42).

**Remote operation**

**Via HART protocol**

**Example: Connection to a HART modem**

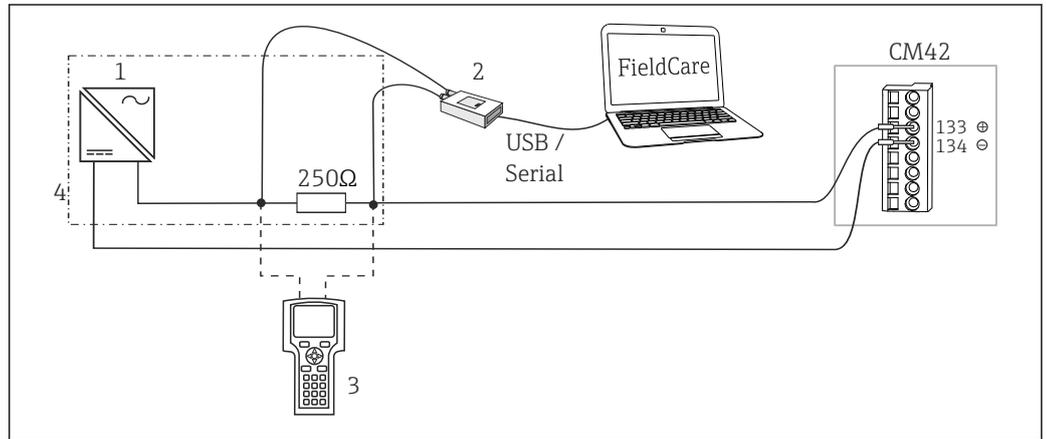


64 HART system integration without PLC

- 1 Power unit 24 V
- 2 HART modem for connection to PC, e.g. FXA195 (switch position "on" substitutes the resistor)
- 3 HART handheld terminal
- 4 Power unit 24 V, with integrated communication load (alternative to 1)

A0032546

Via PROFIBUS-PA

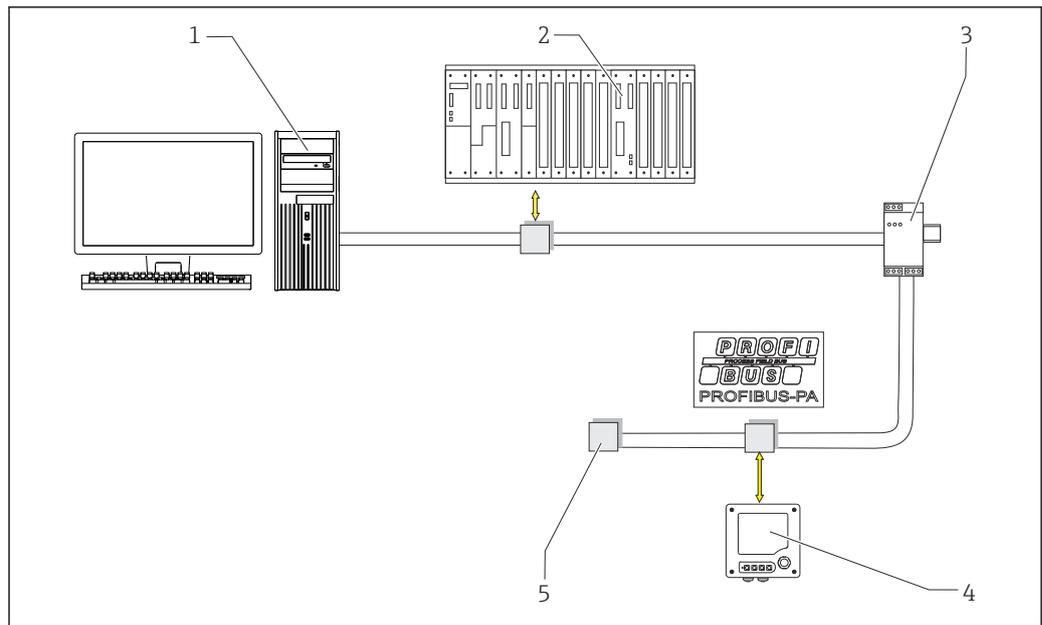


A0032544

65 PROFIBUS system integration

- 1 PC with operating software
- 2 Programmable logic controller (PLC)
- 3 Segment coupler
- 4 Liquiline CM42
- 5 Terminating resistor

Via FOUNDATION Fieldbus

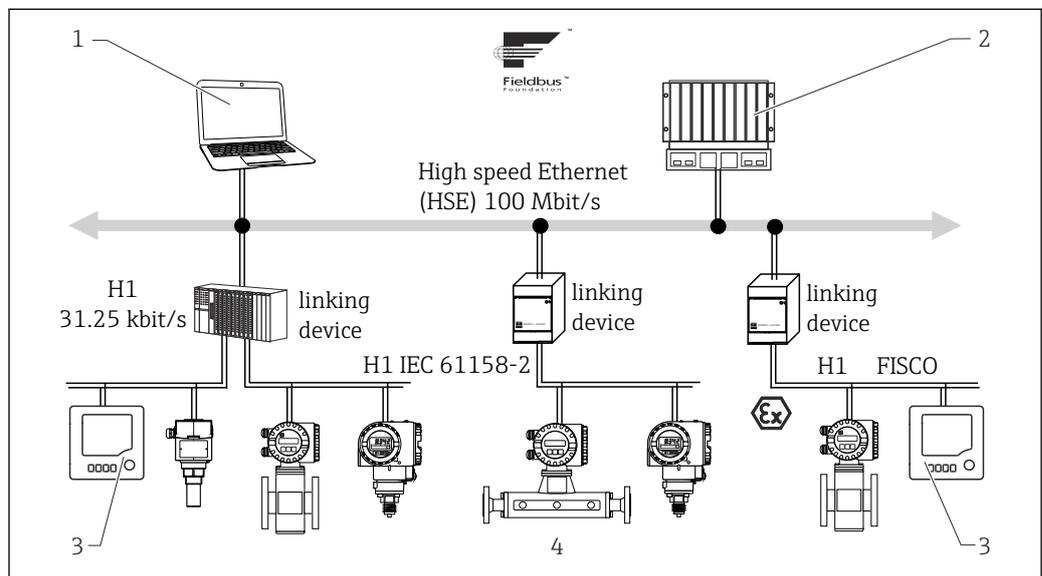

A0032545

66 System architecture with associated components

- 1 Visualization and monitoring, e.g. with FieldCare and diagnostics software
- 2 Field Controller
- 3 Liquiline CM42
- 4 Up to 32 devices per segment

## Certificates and approvals

<b>CE mark</b>	The product meets the requirements of the harmonized European standards. As such, it complies with the legal specifications of the EU directives. The manufacturer confirms successful testing of the product by affixing to it the <b>CE</b> mark.
<b>Hazardous area approvals</b>	Depending on version: <ul style="list-style-type: none"> <li>▪ ATEX II (1)2G Ex ib [ia Ga] IIC T4/T6 Gb / II 3 D Ex tc IIIC T85°C Dc</li> <li>▪ ATEX II (1)2G Ex ib [ia Ga] IIC T4/T6 Gb</li> <li>▪ ATEX II 3D Ex tc [ic IIC Gc] IIIC T85°C Dc</li> <li>▪ ATEX II 3G Ex nA [ic Gc] IIC T4/T6 Gc</li> <li>▪ NEPSI Ex nA [ia Ga] IIC T6 Gc</li> <li>▪ NEPSI Ex ib [ia Ga] IIC T4/T6 Gb</li> <li>▪ CSA IS NI Cl.I, II, III, Div. 1&amp;2, Gr. A-G</li> <li>▪ FM IS NI Cl.I, Div. 1&amp;2, Gr. A-D</li> <li>▪ JPN Ex ib [ia Ga] IIC T6 Gb</li> <li>▪ EAC Ex, 1Ex ib [ia Ga] IIC T6/T4 Gb Zone 1, connected sensors in Zone 0 Certificate number: TC RU C-DE.AA87.B.00088</li> </ul>
<b>Test reports</b>	A test certificate 3.1 in accordance with EN 10204 is supplied depending on the version (→ Product Configurator on the product page).
<b>Other standards and guidelines</b>	The product has been certified according to guidelines TP TC 004/2011 and TP TC 020/2011 which apply in the European Economic Area (EEA). The EAC conformity mark is affixed to the product.

## Ordering information

<b>Product page</b>	<a href="http://www.endress.com/cm42">www.endress.com/cm42</a>
<b>Product Configurator</b>	<p>On the product page there is a <b>Configure</b> button to the right of the product image.</p> <ol style="list-style-type: none"> <li>1. Click this button. <ul style="list-style-type: none"> <li>↳ The Configurator opens in a separate window.</li> </ul> </li> <li>2. Select all the options to configure the device in line with your requirements. <ul style="list-style-type: none"> <li>↳ In this way, you receive a valid and complete order code for the device.</li> </ul> </li> <li>3. Export the order code as a PDF or Excel file. To do so, click the appropriate button on the right above the selection window.</li> </ol> <p> For many products you also have the option of downloading CAD or 2D drawings of the selected product version. Click the <b>CAD</b> tab for this and select the desired file type using picklists.</p>

<b>Scope of delivery</b>	<p>The scope of delivery comprises:</p> <ul style="list-style-type: none"> <li>▪ 1 transmitter in the version ordered</li> <li>▪ 1 mounting plate incl. 4 flat head screws</li> <li>▪ 1 set of adhesive labels (nameplate, terminal connection signs)</li> <li>▪ 1 test certificate according to EN 10204-3.1 (optional)</li> <li>▪ Operating Instructions Part 1 and 2, BA00381C and BA00382C, in the language ordered</li> <li>▪ 1 manufacturer's certificate</li> </ul>
--------------------------	--

## Accessories

The following are the most important accessories available at the time this documentation was issued.

- ▶ For accessories not listed here, please contact your Service or Sales Center.

## Device-specific accessories

**Mounting kits****Post retainer for plastic housing**

- 1 mounting plate
- 2 threaded bolts M5x75 mm A2
- 2 hexagonal nuts M5 A2, DIN 934
- 2 spring washers A2 DIN127, form B5 (M5)
- 2 washers A 5.3, DIN125 A2
- Order No. 51518263

**Post retainer for stainless steel housing**

- 1 mounting plate
- 2 threaded bolts M5x75 mm A2
- 2 hexagonal nuts M5 A2, DIN 934
- 2 spring washers A2 DIN127, form B5 (M5)
- 2 washers A 5.3, DIN125 A2
- Order No. 51518286

**Panel mounting set for plastic housing**

For panel cutout 138x138 mm (5.43x5.43 inch)

- 1 panel mounting seal
- 2 tensioning screws M6x150 mm
- 4 hexagonal nuts M6, DIN934 A2
- 4 spring washers, A2 DIN127, form B6
- 4 washers A6.4, DIN125 A2
- Order No. 51518173

**Panel mounting set for stainless steel housing**

For panel cutout 138x138 mm (5.43x5.43 inch)

- 1 panel mounting seal
- 2 tensioning screws M6x150 mm
- 4 hexagonal nuts M6, DIN934 A2
- 4 spring washers, A2 DIN127, form B6
- 4 washers A6.4, DIN125 A2
- Order No. 51518284

**Weather protection cover****Weather protection cover for plastic housing**

Order number: 51517382

**Weather protection cover for stainless steel housing**

Order number: CYY101-A

**Measuring cable****Memosens data cable CYK10**

- For digital sensors with Memosens technology
- Product Configurator on the product page: [www.endress.com/cyk10](http://www.endress.com/cyk10)



Technical Information TI00118C

**Memosens data cable CYK11**

- Extension cable for digital sensors with Memosens protocol
- Product Configurator on the product page: [www.endress.com/cyk11](http://www.endress.com/cyk11)



Technical Information TI00118C

**Measuring cable CPK9**

- Terminated measuring cable for connecting analog sensors with TOP68 plug-in head
- Selection in accordance with product structure
- Product Configurator on the product page: [www.endress.com/cpk9](http://www.endress.com/cpk9).



Technical Information TI00118C

**Measuring cable CPK12**

- Terminated measuring cable for connecting analog ISFET sensors with TOP68 plug-in head
- Selection in accordance with product structure
- Ordering information: Endress+Hauser sales office or [www.endress.com](http://www.endress.com)

**Measuring cable CYK71**

- Unterminated cable for connecting analog sensors and for extending sensor cables
- Sold by the meter, order numbers:
  - Non-Ex version, black: 50085333
  - Ex-version, blue: 50085673

**Measuring cable CLK6**

- Extension cable for inductive conductivity sensors, for extension via VBM junction box
- Sold by the meter, order number: 71183688

**Sensors**

*Glass electrodes*

**Memosens CPS11E**

- pH sensor for standard applications in process and environmental engineering
- Digital with Memosens 2.0 technology
- Product Configurator on the product page: [www.endress.com/cps11e](http://www.endress.com/cps11e)

 Technical Information TI01493C

**Memosens CPS41E**

- pH sensor for process technology
- With ceramic junction and KCl liquid electrolyte
- Digital with Memosens 2.0 technology
- Product Configurator on the product page: [www.endress.com/cps41e](http://www.endress.com/cps41e)

 Technical Information TI01495C

**Memosens CPS71E**

- pH sensor for chemical process applications
- With ion trap for poison-resistant reference
- Digital with Memosens 2.0 technology
- Product Configurator on the product page: [www.endress.com/cps71e](http://www.endress.com/cps71e)

 Technical Information TI01496C

**Memosens CPS91E**

- pH sensor for heavily polluted media
- With open aperture
- Digital with Memosens 2.0 technology
- Product Configurator on the product page: [www.endress.com/cps91e](http://www.endress.com/cps91e)

 Technical Information TI01497C

**Orbisint CPS11D / CPS11**

- pH sensor for process technology
- With dirt-repellent PTFE diaphragm
- Product Configurator on the product page: [www.endress.com/cps11d](http://www.endress.com/cps11d) or [www.endress.com/cps11](http://www.endress.com/cps11)

 Technical Information TI00028C

**Memosens CPS31D**

- pH electrode with gel-filled reference system with ceramic diaphragm
- Product Configurator on the product page: [www.endress.com/cps31d](http://www.endress.com/cps31d)

 Technical Information TI00030C

**Ceraliquid CPS41D / CPS41**

- pH electrode with ceramic junction and KCl liquid electrolyte
- Product Configurator on the product page: [www.endress.com/cps41d](http://www.endress.com/cps41d) or [www.endress.com/cps41](http://www.endress.com/cps41)

 Technical Information TI00079C

**Ceragel CPS71D / CPS71**

- pH electrode with reference system including ion trap
- Product Configurator on the product page: [www.endress.com/cps71d](http://www.endress.com/cps71d) or [www.endress.com/cps71](http://www.endress.com/cps71)

 Technical Information TI00245C

**Memosens CPS171D**

- pH electrode for bio-fermenters with digital Memosens technology
- Product Configurator on the product page: [www.endress.com/cps171d](http://www.endress.com/cps171d)



Technical Information TI01254C

**Orbipore CPS91D / CPS91**

- pH electrode with open aperture for media with high dirt load
- Product Configurator on the product page: [www.endress.com/cps91d](http://www.endress.com/cps91d) or [www.endress.com/cps91](http://www.endress.com/cps91)



Technical Information TI00375C

**Orbipac CPF81D**

- Compact pH sensor for installation or immersion operation
- In industrial water and wastewater
- Product Configurator on the product page: [www.endress.com/cpf81d](http://www.endress.com/cpf81d)



Technical Information TI00191C

*Enamel pH electrodes***Ceramax CPS341D**

- pH electrode with pH-sensitive enamel
- Meets highest demands of measuring accuracy, pressure, temperature, sterility and durability
- Product Configurator on the product page: [www.endress.com/cps341d](http://www.endress.com/cps341d)



Technical Information TI00468C

*ORP sensors***Memosens CPS12E**

- ORP sensor for standard applications in process and environmental engineering
- Digital with Memosens 2.0 technology
- Product Configurator on the product page: [www.endress.com/cps12e](http://www.endress.com/cps12e)



Technical Information TI01494C

**Orbisint CPS12D / CPS12**

- ORP sensor for process technology
- Product Configurator on the product page: [www.endress.com/cps12d](http://www.endress.com/cps12d) or [www.endress.com/cps12](http://www.endress.com/cps12)



Technical Information TI00367C

**Ceraliquid CPS42D / CPS42**

- ORP electrode with ceramic junction and KCl liquid electrolyte
- Product Configurator on the product page: [www.endress.com/cps42d](http://www.endress.com/cps42d) or [www.endress.com/cps42](http://www.endress.com/cps42)



Technical Information TI00373C

**Ceragel CPS72D / CPS72**

- ORP electrode with reference system including ion trap
- Product Configurator on the product page: [www.endress.com/cps72d](http://www.endress.com/cps72d) or [www.endress.com/cps72](http://www.endress.com/cps72)



Technical Information TI00374C

**Orbipac CPF82D**

- Compact ORP sensor for installation or immersion operation in process water and wastewater
- Product Configurator on the product page: [www.endress.com/cpf82d](http://www.endress.com/cpf82d)



Technical Information TI00191C

**Orbipore CPS92D / CPS92**

- ORP electrode with open aperture for media with high dirt load
- Product Configurator on the product page: [www.endress.com/cps92d](http://www.endress.com/cps92d) or [www.endress.com/cps92](http://www.endress.com/cps92)



Technical Information TI00435C

*pH ISFET sensors*

**Memosens CPS47D**

- Sterilizable and autoclavable ISFET sensor for pH measurement
- Refillable KCl liquid electrolyte
- Product Configurator on the product page: [www.endress.com/cps47d](http://www.endress.com/cps47d)



Technical Information TI01412C

**Memosens CPS77D**

- Sterilizable and autoclavable ISFET sensor for pH measurement
- Product Configurator on the product page: [www.endress.com/cps77d](http://www.endress.com/cps77d)



Technical Information TI01396

**Memosens CPS97D**

- ISFET sensor for pH measurement with long-term stability in media with high dirt loads
- Product Configurator on the product page: [www.endress.com/cps97d](http://www.endress.com/cps97d)



Technical Information TI01405C

*pH and ORP combined sensors*

**Memosens CPS16D**

- Combined pH/ORP sensor for process technology
- With dirt-repellent PTFE diaphragm
- With Memosens technology
- Product Configurator on the product page: [www.endress.com/cps16d](http://www.endress.com/cps16d)



Technical Information TI00503C

**Memosens CPS76D**

- Combined pH/ORP sensor for process technology
- Hygienic and sterile applications
- With Memosens technology
- Product Configurator on the product page: [www.endress.com/cps76d](http://www.endress.com/cps76d)



Technical Information TI00506C

**Memosens CPS96D**

- Combined pH/ORP sensor for chemical processes
- With poison-resistant reference with ion trap
- With Memosens technology
- Product Configurator on the product page: [www.endress.com/cps96d](http://www.endress.com/cps96d)



Technical Information TI00507C

*Conductivity sensors with inductive measurement of conductivity*

**Indumax CLS50D / CLS50**

- High-durability inductive conductivity sensor
- For standard and hazardous area applications
- With Memosens technology
- Product Configurator on the product page: [www.endress.com/cls50d](http://www.endress.com/cls50d) or [www.endress.com/cls50](http://www.endress.com/cls50)



Technical Information TI00182C

**Indumax CLS52**

- Inductive conductivity sensor
- Short response times for the food industry
- Product Configurator on the product page: [www.endress.com/CLS52](http://www.endress.com/CLS52)



Technical Information TI00167C

**Indumax H CLS54D**

- Inductive conductivity sensor
- With certified, hygienic design for foodstuffs, beverages, pharmaceuticals and biotechnology
- Product Configurator on the product page: [www.endress.com/cls54d](http://www.endress.com/cls54d)



Technical Information TI00508C

**Indumax CLS54**

- Inductive conductivity sensor
- For standard and hazardous area applications, available with hygienic design for food, beverages, pharmaceuticals and biotechnology
- Product Configurator on the product page: [www.endress.com/CLS54](http://www.endress.com/CLS54)



Technical Information TI00400C

*Conductivity sensors with conductive measurement of conductivity***Condumax CLS12**

- Conductive conductivity sensor
- For pure water, Ex and high-temperature applications
- Product Configurator on the product page: [www.endress.com/CLS12](http://www.endress.com/CLS12)



Technical Information TI00082C

**Condumax CLS13**

- Conductive conductivity sensor
- For pure water, Ex and high-temperature applications
- Product Configurator on the product page: [www.endress.com/CLS13](http://www.endress.com/CLS13)



Technical Information TI00083C

**Condumax CLS15D / CLS15**

- Conductive conductivity sensor
- For pure water, ultrapure water and hazardous area applications
- Product Configurator on the product page: [www.endress.com/CLS15d](http://www.endress.com/CLS15d) or [www.endress.com/CLS15](http://www.endress.com/CLS15)



Technical Information TI00109C

**Condumax CLS16D / CLS16**

- Hygienic, conductive conductivity sensor
- For pure water, ultrapure water and Ex applications
- With EHEDG and 3A approval
- Product Configurator on the product page: [www.endress.com/CLS16d](http://www.endress.com/CLS16d) or [www.endress.com/CLS16](http://www.endress.com/CLS16)



Technical Information TI00227C

**Condumax CLS19**

- Cost-effective, conductive conductivity sensor
- For applications with pure and ultrapure water
- Product Configurator on the product page: [www.endress.com/CLS19](http://www.endress.com/CLS19)



Technical Information TI00110C

**Condumax CLS21D / CLS21**

- Two-electrode sensor in plug-in head version and fixed cable version
- Product Configurator on the product page: [www.endress.com/CLS21d](http://www.endress.com/CLS21d) or [www.endress.com/CLS21](http://www.endress.com/CLS21)



Technical Information TI00085C

**Memosens CLS82D**

- Four-electrode sensor
- With Memosens technology
- Product Configurator on the product page: [www.endress.com/cls82d](http://www.endress.com/cls82d)



Technical Information TI01188C

*Oxygen sensors*

**Oxymax COS22D**

- Sterilizable sensor for dissolved oxygen
- With Memosens technology
- Product Configurator on the product page: [www.endress.com/cos22d](http://www.endress.com/cos22d)



Technical Information TI00446C

**Oxymax COS51D**

- Amperometric sensor for dissolved oxygen
- With Memosens technology
- Product Configurator on the product page: [www.endress.com/cos51d](http://www.endress.com/cos51d)



Technical Information TI00413C

**Memosens COS81D**

- Sterilizable, optical sensor for dissolved oxygen
- With Memosens technology
- Product Configurator on the product page: [www.endress.com/cos81d](http://www.endress.com/cos81d)



Technical Information TI01201C

---

**Communication-specific accessories**

**Device Care SFE100**

- Configuration of Endress+Hauser devices
- Fast and easy installation, online application updates, one-click connection to devices
- Automatic hardware identification and driver catalog update
- Device configuration with DTMs



Technical Information Device Care SFE100, TI01134S

**Fieldbus connection socket**

- Connection for FOUNDATION Fieldbus M20 7/8"
- Order No. 51517974

**Connector M12**

- Four-pin metal connector for mounting on the transmitter
- For connection to the junction box or cable socket, cable length 150 mm (5.91")
- Order No. 51502184

**C-module accessories kit**

- 1 capacitor for connecting the cable shield to ground potential
- Kit documentation SD00108C
- Order No. 71003097

**Commubox FXA195**

Intrinsically safe HART communication with FieldCare via the USB port



Technical Information TI00404F

**Commubox FXA291**

Connects the CDI interface of measuring devices with the USB port of the computer or laptop



Technical Information TI00405C

**Wireless HART adapter SWA70**

- Wireless device connection
- Easily integrated, offers data protection and transmission safety, can be operated in parallel with other wireless networks, minimum cabling complexity



Technical Information TI00061S

**Field Data Manager Software MS20/21**

- PC software for central data management
- Visualization of series of measurements and logbook events
- SQL database for secure data storage

**FieldCare SFE500**

- Universal tool for field device configuration and management
- Supplied with a complete library of certified DTMs (Device Type Manager) for operation of Endress +Hauser field devices
- Order according to product order structure
- [www.endress.com/sfe500](http://www.endress.com/sfe500)

**Memobase Plus CYZ71D**

- PC software to support laboratory calibration
- Visualization and documentation of sensor management
- Sensor calibrations stored in database
- Product Configurator on the product page: [www.endress.com/cyz71d](http://www.endress.com/cyz71d)



Technical Information TI00502C

**Service-specific accessories****DAT module CY42**

- Function upgrade, update and memory module
- Order numbers:
  - CopyDAT, to save the configuration and copy the configuration to additional devices  
CY42-C1
  - FunctionDAT, to upgrade the function to 2 current outputs  
CY42-F1
  - FunctionDAT, to upgrade the function to "Advanced version"  
CY42-F2
  - SystemDAT, for software updates, extended range of languages  
CY42-S1

**System components****RIA14, RIA16**

- Field display unit for integration into 4-20 mA circuits
- RIA14 in flameproof metal enclosure



Technical Information TI00143R and TI00144R

**RIA15**

- Process display unit, Digital display unit for integration into 4-20 mA circuits
- Panel mounting
- With optional HART communication



Technical Information TI01043K

**Active barrier****Active barrier RN221N**

With power supply for safe separation of 4 to 20 mA standard signal circuits



Technical Information TI00073R

---







71496249

[www.addresses.endress.com](http://www.addresses.endress.com)

---